



NORCE Norwegian Research Centre AS
www.norceresearch.no

REPORT

Handbook for uncertainty calculations for gas flow metering stations

Documentation of uncertainty models and internet tool



Authors

Kjell-Eivind Frøysa, Gaute Øverås Lied

Document Info

Authors

Kjell-Eivind Frøysa, Gaute Øverås Lied

Classification

A - open

Title

Handbook for uncertainty calculations for gas flow metering stations. Documentation of uncertainty models and internet tool.

Extract

The present work is a generalization of the uncertainty models for fiscal gas metering stations in [Lunde et al, 2002] and [Dahl et al, 2003]. The uncertainty models have been made more flexible, allowing gas chromatographs and also gas sampling. In addition to orifice and ultrasonic flow metering stations also Coriolis flow metering stations are covered. Two meters in parallel is covered, and for ultrasonic and Coriolis flow meters also two flow meters in series are covered. The uncertainty models are implemented on two different web-based platforms, one new web application using HTML and WebAssembly, and the original using Microsoft Silverlight technology. These can be accessed for free from nfogm.no.

Project Info

Client

Norwegian Society for Oil and Gas Measurement

Clients ref.

Morten Marstein

NORCE Project No.

101422

NORCE Project Name

Oppgradering av NFOGM usikkerhetsverktøy

Revision

Rev.	Date	Author	Checked by	Approved by	Reason for revision
00	16.06.2020	Kjell-Eivind Frøysa	Gaute Ø. Lied	Ranveig N. Bjørk	

Table of Contents

Disclaimer	7
1 Introduction	8
2 Description of metering stations	10
3 Gas measurement uncertainties	11
3.1 Temperature measurement	11
3.2 Pressure measurement	12
3.3 Differential pressure measurement	13
3.4 Densitometer measurement	14
3.5 Gas composition measurement	16
3.5.1 Gas chromatography measurement	17
3.5.2 Spot sampling and laboratory analysis	17
3.6 Gas quality parameters uncertainty	18
3.6.1 Functional relationship	18
3.6.2 Uncertainty model	19
4 Orifice fiscal metering stations	22
4.1 Description of metering station	22
4.2 Functional relationship	22
4.2.1 General expressions	22
4.2.2 Expressions when densitometer is used	23
4.2.3 Expressions when densitometer is not used	24
4.3 Uncertainty model	24
4.3.1 When densitometer is used	24
4.3.2 When densitometer is not used	25
4.4 Two flow meters in parallel	26
4.4.1 Correlation classification	26
4.4.2 Specific uncertainty models, when densitometer is in use	27
4.4.3 Specific uncertainty models, when densitometer is not in use	29
5 Coriolis fiscal metering station	32
5.1 Description of metering station	32
5.2 Functional relationship	32
5.2.1 Mass flow rate, flow calibrated Coriolis meter	32
5.2.2 Standard volumetric flow rate and energy flow rate, flow calibrated Coriolis meter	33
5.3 Uncertainty model, mass flow rate	33
5.3.1 Calibration uncertainty	33
5.3.2 Field uncertainty	34
5.3.3 Total uncertainty in mass flow rate, one flow meter	35

5.4	Uncertainty model, standard volume and energy flow rate.....	35
5.5	Two flow meters in parallel	36
5.5.1	Correlation classification.....	36
5.5.2	Specific uncertainty models	36
5.6	Two flow meters in series.....	38
5.6.1	Correlation classification.....	39
5.6.2	Specific uncertainty models	39
6	USM fiscal metering stations	42
6.1	Description of metering station	42
6.2	Functional relationship	42
6.2.1	Actual volume flow rate, flow calibrated USM meter	42
6.2.2	Mass, standard volume and energy flow rate, flow calibrated USM meter	43
6.3	Uncertainty model, actual volume flow rate	44
6.3.1	Calibration uncertainty	44
6.3.2	Field uncertainty	45
6.3.3	Total uncertainty in actual volume flow rate, one flow meter	46
6.4	Uncertainty model, mass, standard volume and energy flow rate	46
6.4.1	Densitometer in use.....	47
6.4.2	Densitometer not in use.....	47
6.5	Two flow meters in parallel	48
6.5.1	Correlation classification.....	48
6.5.2	Specific uncertainty model, densitometer in use	49
6.5.3	Specific uncertainty model, densitometer not in use	51
6.6	Two flow meters in series.....	53
6.6.1	Correlation classification.....	53
6.6.2	Specific uncertainty model, densitometer in use	54
6.6.3	Specific uncertainty model, densitometer not in use	56
7	GasMetering Silverlight Application	60
7.1	Software platform	60
7.2	Installation and use	60
7.3	Program overview	60
7.3.1	Specify metering station template	61
7.3.2	Conditions Page	64
7.3.3	Gas Analysis Page	65
7.3.4	Flow Measurement Page.....	68
7.3.5	Uncertainty Calculation Results Page	70
7.3.6	Uncertainty Budget Charts Page	72
7.3.7	Uncertainty Range Plots Page	73

7.3.8	Uncertainty Report Page.....	73
7.3.9	Note about “Save” and “Open” functionality	75
7.3.10	Note about “opening” an uncertainty analysis file.....	75
8	GasMetApp Web Application	76
8.1	Software platform	76
8.2	Installation and use	76
8.3	Program overview	76
8.3.1	Specify metering station template.....	77
8.3.2	Conditions Page.....	79
8.3.3	Gas Analysis Page.....	82
8.3.4	Flow Measurement Page	85
8.3.5	Uncertainty Calculation Results Page	87
8.3.6	Uncertainty Budget Charts Page	89
8.3.7	Uncertainty Report Page.....	90
8.3.8	Note about use of “browser refresh”	91
9	Summary	92
10	References	93
Appendix A	Detailed formulas for uncertainty of correction factor after flow calibration....	95
A 1	Functional relationship	95
A 2	Uncertainty model	97
Appendix B	Uncertainty model for two flow meters in parallel or in series	101
B 1	Generic uncertainty model for one flow meter	101
B 2	Two flow meters in parallel.....	102
B 3	Two flow meters in series.....	104
Appendix C	USM field uncertainty, detailed level	108
Appendix D	List of symbols.....	109

Disclaimer

NORCE is not liable in any form or manner for the actual use of the documents, software or other results made available for or resulting from a project and does not warrant or assume any liability or responsibility for the completeness or usefulness of any information unless specifically agreed otherwise in the tender and resulting contract document.

1 Introduction

Documentation of uncertainty of flow rates measured by fiscal flow metering stations is essential as part of the evaluation of the condition of such metering stations. Authorities have requirements with respect to maximum uncertainty in order to secure the national interests. The partners selling the gas have interests in the uncertainty to secure their incomes. Finally, buyers of gas have interest in ensuring that they are not getting a lower amount of gas than what they pay for.

In order to get all parties to accept an uncertainty analysis, it is important to obtain standardized ways of carrying out such analyses. The ISO Guide to the expression of uncertainty in measurement, [ISO GUM] provides general methodology for carrying out uncertainty analyses. This methodology can also be applied in uncertainty analysis of fiscal gas metering stations. However, the ISO GUM does not give detailed methods for the specific uncertainty analyses for such metering stations (or other applications). Therefore models have to be developed based on the ISO GUM methodology. Similarly the ISO 5168 provides general procedures for evaluation of uncertainty for the measurement of fluid flow. Also the procedures in this standard have to be developed further in order to approach the uncertainty evaluation of a specific metering station.

The Norwegian Society for Oil and Gas Measurement (NFOGM) in cooperation with the Norwegian Petroleum Directorate (NPD) and The Norwegian Society of Graduate Technical and Scientific Professionals (Tekna) have earlier issued Handbooks with uncertainty models for a fiscal ultrasonic gas metering station [Lunde et al, 2002] and a fiscal orifice gas metering station [Dahl et al, 2003]. These works are in agreement with the ISO GUM methodology, and were based on a previous version of the ISO GUM from 1995. The calculation of the uncertainty have in these works been based on an Excel spread sheet that can be downloaded for free from nfogm.no. In addition, uncertainty models for fiscal turbine oil metering stations [Dahl et al, 2003] and fiscal ultrasonic oil metering stations [Lunde et al, 2010] have been established.

The present work is a further development of the uncertainty models for fiscal gas metering stations in [Lunde et al, 2002] and [Dahl et al, 2003]. The intention of this work was to establish an uncertainty analysis model covering the most common fiscal gas metering station configurations in use on the Norwegian Sector. The intention was also to make a tool in which a complete uncertainty analysis for a gas metering station can be performed within one tool in a minimum of time. This is achieved as the tool calculates all necessary parameters from a minimum of inputs, having reasonable default values, having default input values for uncertainty in accordance with requirements in the Norwegian measurement regulations and NORSOK and by making it easy to define the most common metering station configurations in the tool.

The uncertainty model has been made more flexible, allowing gas chromatographs and also gas sampling. In addition to orifice and ultrasonic flow metering stations also Coriolis flow metering stations are covered. Two meters in parallel are covered, and for ultrasonic and Coriolis flow meters also two flow meters in series are covered. The uncertainty models are implemented on two different web-based platforms, one new web application (GasMetApp) using HTML and WebAssembly, and the original (GasMetering) using Microsoft Silverlight technology. Both versions use the same file format. These can be accessed for free from nfogm.no. Since support for the Silverlight runtime will end 12. October 2021, users should transition to the new web application before this date.

This report is a documentation of the uncertainty models developed and the web-based calculation tool. It should be noted that the example input values in that calculation tool are just examples, and should not be regarded as recommended values by NFOGM, NORCE, NPD or any other party.

Chapter 2 of this report describes on an overview level the metering stations covered in the report. In Chapter 3, uncertainties related to secondary instrumentation like temperature pressure, differential pressure, density and gas composition in addition to gas parameters calculated from the gas composition, are covered. Chapter 4 documents the uncertainty model for orifice flow metering stations, Chapter 5 documents the uncertainty model for Coriolis flow metering stations and Chapter 6 documents

the uncertainty model for ultrasonic flow metering stations. Chapter 7 documents the original GasMetering Silverlight application, and Chapter 9 documents the new GasMetApp web application using HTML and WebAssembly. Chapter 9 includes a brief summary of the report.

Appendix A contains some details with respect to the uncertainty model related to adjustments of a flow meter after flow calibration. Appendix B contains the uncertainty model for two flow meters in parallel and series, based on the uncertainty model for a metering station with just one flow meter. Appendix C provides the detailed link between this report and the previous work [Lunde et al, 2002] that the uncertainty model for the ultrasonic flow meters is based on. Appendix D contains a list of symbols.

The uncertainty models presented here are based on the ISO GUM uncertainty methodology. The measurement regulations by the Norwegian Petroleum Directorate and the NORSOK standard I-106 and I-104 on fiscal measurement systems for hydrocarbon gas [NORSOKI-106, NORSOK I-104] have been important references with respect to layout of the meter stations and requirements to the uncertainty of individual instruments and the operation of the metering station as a whole. A series of ISO and other international standards and reports have also been essential in this work. The details are covered in the relevant sections of the report. It is also referred to the reference list in Chapter 10.

The present work has been carried out for Norwegian Society for Oil and Gas Measurement (NFOGM) with financial support also from Norwegian Petroleum Directorate and Tekna. A reference group consisting of the following members has followed the work:

- Dag Flølo, Statoil and NFOGM
- Rune Andersen, Norwegian Environment Agency
- Sidsel Corneliussen, BP
- Leif Einar Falnes, Shell
- Endre Jacobsen, Statoil
- Pål Jaghø, Talisman Energy
- Svein Neumann, Conoco Phillips
- Anfinn Paulsen, Gassco
- Reidar Sakariassen, MetroPartner
- Bjarne Syre, DONG Energy
- Steinar Vervik, Norwegian Petroleum Directorate
- Kjell Arne Ulvund, Statoil

Dag Flølo has been especially involved with regular project meetings and discussions throughout the project.

2 Description of metering stations

In the present Handbook, several metering configurations of metering stations are covered. These include

- Orifice plate metering stations
- Coriolis metering stations
- Ultrasonic flow metering stations

The following three configurations are addressed:

- One flow meter (orifice, ultrasonic or Coriolis)
- Two flow meters in parallel (orifice, ultrasonic or Coriolis)
- Two flow meters in series (ultrasonic or Coriolis)

With respect to gas quality, three configurations are covered:

- Densitometer (in addition to a “nominal” gas composition)
- Online gas chromatography
- Gas sampling and laboratory analysis at regular time intervals

When the orifice metering station is selected, no flow calibration is involved. The uncertainty analysis of the orifice metering station follows the ISO 5167 as for the previous handbook [Dahl et al, 2003].

The Coriolis flow meter is assumed to be flow calibrated. The uncertainty model for this type of meter will not focus on flow meter technology details, but will be kept on an overall level. ISO 10970, including the amendment, is the recognized international standard for Coriolis fiscal gas metering.

The ultrasonic flow meter is also assumed to be flow calibrated. The uncertainty model is similar to the model in the previous handbook [Lunde et al, 2002], but with necessary generalizations due to metering station setup. ISO 17089-1 is the recognized international standard for ultrasonic fiscal gas metering.

3 Gas measurement uncertainties

This chapter will address the uncertainty models for the measurements of temperature (Section 3.1), pressure (Section 3.2), differential pressure (Section 3.3), density (Section 3.4) and gas compositions (Section 3.5), in addition to the uncertainty of standard density, calorific value and CO₂ emission factor, as calculated from a gas composition (Section 3.6).

3.1 Temperature measurement

The uncertainty model for the temperature measurement follows the similar model in [Lunde et al, 2002] and [Dahl et al, 2003].

The uncertainty in the measured temperature can be specified in two ways:

- Overall level
- Detailed level

In case of the overall level, the absolute uncertainty in the measured temperature is specified directly by the user of the uncertainty calculation program.

In case of the detailed level, the following uncertainty model is used:

$$u(T)^2 = u(T_{elem,transm})^2 + u(T_{stab,transm})^2 + u(T_{RFI})^2 + u(T_{temp})^2 + u(T_{stab,elem})^2 + u(T_{misc})^2, \quad (3.1)$$

where

- $u(T_{elem,transm})$: standard uncertainty of the temperature element and temperature transmitter, calibrated as a unit. Typically found either in product specifications or in calibration certificates.
- $u(T_{stab,transm})$: standard uncertainty related to the stability of the temperature transmitter, with respect to drift in readings over time. Typically found in product specifications.
- $u(T_{RFI})$: standard uncertainty due to radio-frequency interference (RFI) effects on the temperature transmitter.
- $u(T_{temp})$: standard uncertainty of the effect of temperature on the temperature transmitter, for change of gas temperature relative to the temperature at calibration. Typically found in product specifications.
- $u(T_{stab,elem})$: standard uncertainty related to the stability of the temperature element. Instability may relate e.g. to drift during operation, as well as instability and hysteresis effects due to oxidation and moisture inside the encapsulation, and mechanical stress during operation. Typically found in product specifications.
- $u(T_{misc})$: standard uncertainty of other (miscellaneous) effects on the temperature transmitter.

This uncertainty model is quite generic, and can be used on a series of industrial products. In cases where this model does not fit with the product specifications, the miscellaneous uncertainty contributions can be used for specification of other uncertainty contributions. Alternatively, the uncertainty of the temperature measurements can be calculated manually, and the result can be given to the program using the overall input level.

When the average of two temperature measurements is used, it is assumed that the two temperature measurements are uncorrelated. The reason for this assumption is that often the two probes are not calibrated at the same time. This means that even if they are calibrated using the same procedure, the time difference generates an uncorrelated drifting term, both in the reference and in the temperature measurement itself. This means that the uncertainty in the average of two temperature measurements is assumed to be equal to the uncertainty for one measurement, divided by the square root of two.

3.2 Pressure measurement

The uncertainty model for the pressure measurement follows the similar model in [Lunde et al, 2002] and [Dahl et al, 2003].

The uncertainty in the measured pressure can be specified in two ways:

- Overall level
- Detailed level

In case of the overall level, the relative uncertainty in the measured pressure is specified directly by the user of the uncertainty calculation program.

In case of the detailed level, the following uncertainty model is used:

$$u(P)^2 = u(P_{transmitte})^2 + u(P_{stability})^2 + u(P_{RFI})^2 + u(P_{temp})^2 + u(P_{atm})^2 + u(P_{misc})^2, \quad (3.2)$$

where

- $u(P_{transmitte})$: standard uncertainty of the pressure transmitter, including hysteresis, terminal-based linearity, repeatability and the standard uncertainty of the pressure calibration laboratory.
- $u(P_{stability})$: standard uncertainty of the stability of the pressure transmitter, with respect to drift in readings over time.
- $u(P_{RFI})$: standard uncertainty due to radio-frequency interference (RFI) effects on the pressure transmitter.
- $u(P_{temp})$: standard uncertainty of the effect of ambient gas temperature on the pressure transmitter, for change of ambient temperature relative to the temperature at calibration.
- $u(P_{atm})$: standard uncertainty of the atmospheric pressure, relative to 1 atm. = 1.01325 bar, due to local meteorological effects. This effect is of relevance for units measuring gauge pressure.
- $u(P_{misc})$: standard uncertainty due to other (miscellaneous) effects on the pressure transmitter, such as mounting effects, etc.

This uncertainty model is quite generic, and can be used on a series of industrial products. In cases where this model does not fit with the product specifications, the miscellaneous uncertainty contributions can be used for specification of other uncertainty contributions. Alternatively, the uncertainty of the pressure measurements can be calculated manually, and the result can be given to the program using the overall input level.

When the average of two pressure measurements is used, it is assumed that the two pressure measurements are uncorrelated. The reason for this assumption is that often the two probes are not calibrated at the same time. This means that even if they are calibrated using the same procedure, the time difference generates an uncorrelated drifting term, both in the reference and in the pressure measurement itself. This means that the uncertainty in the average of two pressure measurements is assumed to be equal to the uncertainty for one measurement, divided by the square root of two.

3.3 Differential pressure measurement

The uncertainty model for the differential pressure measurement follows the similar model in [Dahl et al, 2003].

The uncertainty in the measured differential pressure can be specified in two ways:

- Overall level
- Detailed level

In case of the overall level, the absolute uncertainty in the measured differential pressure is specified directly by the user of the uncertainty calculation program.

In case of the detailed level, the following uncertainty model is used:

$$u(\Delta P)^2 = u(\Delta P_{transmitte})^2 + u(\Delta P_{stability})^2 + u(\Delta P_{RFI})^2 + u(\Delta P_{temp})^2 + u(\Delta P_{misc})^2, \quad (3.3)$$

where

- $u(\Delta P_{transmitte})$: standard uncertainty of the differential pressure transmitter, including hysteresis, terminal-based linearity, repeatability and the standard uncertainty of the differential pressure calibration laboratory.
- $u(\Delta P_{stability})$: standard uncertainty of the stability of the differential pressure transmitter, with respect to drift in readings over time.
- $u(\Delta P_{RFI})$: standard uncertainty due to radio-frequency interference (RFI) effects on the differential pressure transmitter.
- $u(\Delta P_{temp})$: standard uncertainty of the effect of ambient gas temperature on the differential pressure transmitter, for change of ambient temperature relative to the temperature at calibration.
- $u(\Delta P_{misc})$: standard uncertainty due to other (miscellaneous) effects on the differential pressure transmitter, such as mounting effects, etc.

This uncertainty model is quite generic, and can be used on a series of industrial products. In cases where this model does not fit with the product specifications, the miscellaneous uncertainty contributions can be used for specification of other uncertainty contributions. Alternatively, the uncertainty of the differential pressure measurements can be calculated manually, and the result can be given to the program using the overall input level.

3.4 Densitometer measurement

The uncertainty model for the density measurement follows the similar model in [Lunde et al, 2002] and [Dahl et al, 2003].

The uncertainty in the measured density can be specified in two ways:

- Overall level
- Detailed level

In case of the overall level, the relative uncertainty in the measured density is specified directly by the user of the uncertainty calculation program.

In case of the detailed level, the uncertainty model is more complicated than for the temperature, pressure and differential pressure measurements above. The density measurement consists of several steps:

- Measurement of an uncorrected density from the period measurement of a vibrating string.
- Corrections based on temperature difference between calibration and measurement.
- Velocity of sound corrections.
- Corrections for pressure and temperature differences from the densitometer to the line conditions.

This will in total form the functional relationship for the density measurement, in agreement with ISO 15970, as follows:

$$\rho = \left\{ \rho_u \left[1 + K_{18}(T_d - T_c) \right] + K_{19}(T_d - T_c) \right\} \frac{1 + \left(\frac{K_d}{\tau_c} \right)^2}{1 + \left(\frac{K_d}{\tau_d} \right)^2} \left(\frac{T_d}{T} \right) \left(\frac{1}{1 + \Delta P_d / P} \right) \left(\frac{Z_d}{Z} \right) . \quad (3.4)$$

In this equation subscript “d” means densitometer conditions and subscript “c” means calibration conditions. The following variables are used in this equation:

ρ_u :	indicated (uncorrected) density, in density transducer [kg/m ³].
K_{18}, K_{19} :	constants from the calibration certificate.
T_d :	gas temperature in density transducer [K].
T_c :	calibration temperature [K].
K_d :	transducer constant [μm] (square root of constant K_d in ISO 15970).
c_c :	VOS for the calibration gas, at calibration temperature and pressure conditions [m/s].
c_d :	VOS for the measured gas, in the density transducer [m/s].
τ :	periodic time (inverse of the resonance frequency, output from the densitometer) [μs].
T :	gas temperature in the pipe, at the flow meter location (line conditions) [K].
P :	gas pressure in the pipe, at the flow meter location (line conditions) [bara].
ΔP_d :	pressure difference between the line and densitometer pressures (usually negative) [bara].
Z_d :	gas compressibility factor for the gas in the density transducer.
Z :	gas compressibility factor for the gas in the pipe, at orifice location (line conditions).

By using the general uncertainty model approach in ISO GUM [ISO GUM, 2008], the uncertainty model will be

$$\begin{aligned}
u_c^2(\rho) = & s_{\rho_u}^2 u^2(\rho_u) + u^2(\rho_{rept}) + s_{\rho,T}^2 u_c^2(T) + s_{\rho,T_d}^2 u^2(T_d) + s_{\rho,T_c}^2 u^2(T_c) \\
& + s_{\rho,K_d}^2 u^2(K_d) + s_{\rho,\tau}^2 u^2(\tau) + s_{\rho,c_c}^2 u^2(c_c) + s_{\rho,c_d}^2 u^2(c_d) \\
& + s_{\rho,\Delta P_d}^2 u^2(\Delta P_d) + s_{\rho,P}^2 u^2(P) + u^2(\rho_{temp}) + u^2(\rho_{misc}),
\end{aligned} \tag{3.5}$$

where

- $u(\rho_u)$: standard uncertainty of the indicated (uncorrected) density estimate, ρ_u , including the calibration laboratory uncertainty, the reading error during calibration, and hysteresis.
- $u(\rho_{rept})$: standard uncertainty of the repeatability of the indicated (uncorrected) density estimate, ρ_u .
- $u(T)$: standard uncertainty of the line temperature estimate, T .
- $u(T_d)$: standard uncertainty of the gas temperature estimate in the densitometer, T_d .
- $u(T_c)$: standard uncertainty of the densitometer calibration temperature estimate, T_c .
- $u(K_d)$: standard uncertainty of the VOS correction densitometer constant estimate, K_d .
- $u(\tau)$: standard uncertainty of the periodic time estimate, τ .
- $u(c_c)$: standard uncertainty of the calibration gas VOS estimate, c_c .
- $u(c_d)$: standard uncertainty of the densitometer gas VOS estimate, c_d .
- $u(\Delta P_d)$: standard uncertainty of assuming that $P_d = P$, due to possible deviation of gas pressure from densitometer to line conditions.
- $u(P)$: standard uncertainty of the line pressure estimate, P .
- $u(\rho_{temp})$: standard uncertainty of the temperature correction factor for the density estimate, ρ (represents the *model uncertainty* of the temperature correction model used, $\{\rho_u [1 + K_{18}(T_d - T_c)] + K_{19}(T_d - T_c)\}$).
- $u(\rho_{misc})$: standard uncertainty of the density estimate, accounting for miscellaneous uncertainty contributions, such as due to:
- stability (drift, shift between calibrations),
 - reading error during measurement (for digital display instruments),
 - possible deposits on the vibrating element,
 - possible corrosion of the vibrating element,
 - possible liquid condensation on the vibrating element,
 - mechanical (structural) vibrations on the gas line,
 - variations in power supply,
 - self-induced heat,
 - flow in the bypass density line,
 - possible gas viscosity effects,
 - neglecting possible pressure dependency in calculation of the uncorrected density from the periodic time,
 - model uncertainty of the VOS correction model,
 - other possible effects.

The sensitivity coefficients in Eq. (3.5) can be calculated from the functional relationship Eq. (3.4) by use of the ISO GUM methodology:

$$s_{\rho_u} = \frac{\partial \rho}{\partial \rho_u} = \frac{\rho [1 + K_{18}(T_d - T_c)]}{\rho_u [1 + K_{18}(T_d - T_c)] + K_{19}(T_d - T_c)} \tag{3.6}$$

$$s_{\rho,T} = \frac{\partial \rho}{\partial T} = -\frac{\rho}{T} \quad (3.7)$$

$$s_{\rho,T_d} = \frac{\partial \rho}{\partial T_d} = \left[1 + \frac{T_d [\rho_u K_{18} + K_{19}]}{\rho_u [1 + K_{18}(T_d - T_c)] + K_{19}(T_d - T_c)} \right] \frac{\rho}{T_d} \quad (3.8)$$

$$s_{\rho,T_c} = \frac{\partial \rho}{\partial T_c} = - \left[\frac{T_c [\rho_u K_{18} + K_{19}]}{\rho_u [1 + K_{18}(T_d - T_c)] + K_{19}(T_d - T_c)} \right] \frac{\rho}{T_c} \quad (3.9)$$

$$s_{\rho,K_d} = \frac{\partial \rho}{\partial K_d} = \left[\frac{2K_d^2}{K_d^2 + (\pi_c)^2} - \frac{2K_d^2}{K_d^2 + (\pi_d)^2} \right] \frac{\rho}{K_d} \quad (3.10)$$

$$s_{\rho,\tau} = \frac{\partial \rho}{\partial \tau} = - \left[\frac{2K_d^2}{K_d^2 + (\pi_c)^2} - \frac{2K_d^2}{K_d^2 + (\pi_d)^2} \right] \frac{\rho}{\tau} \quad (3.11)$$

$$s_{\rho,c_c} = \frac{\partial \rho}{\partial c_c} = - \frac{2K_d^2}{K_d^2 + (\pi_c)^2} \frac{\rho}{c_c}; \quad s_{\rho,c_d} = \frac{\partial \rho}{\partial c_d} = \frac{2K_d^2}{K_d^2 + (\pi_d)^2} \frac{\rho}{c_d} \quad (3.12)$$

$$s_{\rho,\Delta P_d} = \frac{\partial \rho}{\partial \Delta P_d} = - \frac{\rho}{P + \Delta P_d}; \quad s_{\rho,P} = \frac{\partial \rho}{\partial P} = \frac{\Delta P_d}{P + \Delta P_d} \frac{\rho}{P} \quad (3.13)$$

3.5 Gas composition measurement

In this section, first the uncertainty model for the individual gas components resulting from an online gas chromatography measurement is presented in Section 3.5.1. Thereafter uncertainty model for individual gas components related to spot sampling and laboratory analysis is presented in Section 3.5.2.

3.5.1 Gas chromatography measurement

NORSOK I-106 states the following uncertainty contributions for the molar fractions of the various gas components as measured by an online gas chromatograph:

- Repeatability
- Linearity
- Calibration gas uncertainty

This means that the standard uncertainty of the measured molar fraction ϕ_i of gas component number i can be written as

$$u(\phi_i)^2 = u(\phi_{i, rept})^2 + u(\phi_{i, lin})^2 + u(\phi_{i, cal})^2, \quad (3.14)$$

where

- $u(\phi_i)$: standard uncertainty of the measured molar fraction of gas component number i .
- $u(\phi_{i, rept})$: standard uncertainty due to repeatability, of the measured molar fraction of gas component number i .
- $u(\phi_{i, lin})$: standard uncertainty due to linearity, of the measured molar fraction of gas component number i .
- $u(\phi_{i, cal})$: standard uncertainty due to calibration gas uncertainty, of the measured molar fraction of gas component number i .

3.5.2 Spot sampling and laboratory analysis

In the case of gas composition estimation from spot sampling and laboratory analysis, the uncertainty in the average gas composition over a time period (for example one year) is calculated. The standard uncertainty in the average value of the molar fraction of gas component number i is found as

$$u(\phi_i)^2 = u(\phi_{i, sampling})^2 + u(\phi_{i, analysis})^2 + u(\phi_{i, frequency})^2, \quad (3.15)$$

where

- $u(\phi_i)$: standard uncertainty of the average measured molar fraction of gas component number i .
- $u(\phi_{i, sampling})$: standard uncertainty due to representativity of the gas sampling of gas component number i .
- $u(\phi_{i, analysis})$: standard uncertainty related to analyzer uncertainty at laboratory of gas component number i .
- $u(\phi_{i, frequency})$: standard uncertainty due to fluctuations in the values for gas component number i , between the samples taken over the time period (e.g. a year). Therefore it is related to the number of samples, i.e. the sampling frequency.

The standard uncertainty due to sampling will have to be given as input in the program. No automatic estimation of this quantity is carried out.

The standard uncertainty related to analyzer uncertainty is treated in the same way as the gas chromatography uncertainty presented in Section 3.5.1, Eq. (3.14).

The standard uncertainty related to sampling frequency is calculated as

$$u(\phi_{i, frequency}) = \frac{T\sigma_i}{2\sqrt{N}}, \quad (3.16)$$

where

N : number of gas samples
 T : Student-T parameter for 95 % confidence level ($T.INV.2T(0.05;N-1)$ in Excel)
 σ_i : standard deviation over the gas samples of molar fractions measured for gas component number i

3.6 Gas quality parameters uncertainty

This section describes the general approach for uncertainty analysis of gas quality parameters. Section 3.6.1 covers the functional relationships, and Section 3.6.2 the uncertainty model.

3.6.1 Functional relationship

In general, the functional relationship for a gas parameter, X , can be written

$$X = f(\phi_1, \phi_2, \dots, \phi_n, P, T), \quad (3.17)$$

where $\phi_1, \phi_2, \dots, \phi_n$ are un-normalized molar fractions for each gas component. Note that in the function calculating the gas parameter, a normalization of the gas composition is included (i.e. to divide each of the molar fractions by the sum of all molar fractions to ensure that the sum of all molar fractions then will be equal to 1).

A series of gas quality parameters can be calculated from the gas composition alone using the algorithms in ISO 6976. This includes e.g. molar mass (m), compressibility factor at standard conditions (Z_0), mass based superior calorific value ($H_{s,m}$) and mass based inferior calorific value ($H_{l,m}$). The compressibility factor at line conditions (Z) can be calculated from the gas composition in combination with the pressure and temperature by use of the algorithms in AGA 8. The CO₂ emission factor can also be calculated from the gas composition. There are no recognized international standard for this parameter. X can represent each of these gas parameters, and also combinations (like ratios and products etc.) of them.

The CO₂ emission factor is calculated using the following formulas:

Mass based CO₂ emission factor (kg/kg):

$$C_m = m_{CO_2} \frac{\sum_{i=1}^n n_i \phi_i}{\sum_{i=1}^n m_i \phi_i}, \quad (3.18)$$

where m_{CO_2} is the molar mass of CO₂, n_i is the number of carbon atoms in the molecule for gas component number i and m_i is the molar mass of gas component number i .

Volume based CO₂ emission factor (kg/Sm³):

$$C_v = C_m \rho_0, \quad (3.19)$$

where ρ_0 is the density at standard conditions, calculated from the gas composition by use of ISO 6976.

Energy based CO₂ emission factor (tonnes/TJ):

$$C_e = 1000 C_m / H_{I,m}, \quad (3.20)$$

where $H_{I,m}$ is the mass based inferior calorific value (MJ/kg), calculated from the gas composition by use of ISO 6976.

3.6.2 Uncertainty model

Uncertainty in the gas components and in pressure and temperature will generate uncertainty in the gas parameters. The standard uncertainty of each gas parameter X can now be found as

$$u(X)^2 = \left(\frac{\partial f}{\partial \phi_1} u(\phi_1) \right)^2 + \left(\frac{\partial f}{\partial \phi_2} u(\phi_2) \right)^2 + \dots + \left(\frac{\partial f}{\partial \phi_n} u(\phi_n) \right)^2 + \left(\frac{\partial f}{\partial P} u(P) \right)^2 + \left(\frac{\partial f}{\partial T} u(T) \right)^2 + (u(X_{\text{model}}))^2. \quad (3.21)$$

The last term in this uncertainty model represents a possible model uncertainty due to approximations and inaccuracies in Eq. (3.17).

Some of the functional relationships, Eq. (3.17), are quite complex, and analytic calculation of the partial derivatives is complicated. Therefore, the partial derivatives are calculated numerically as

$$\frac{\partial f}{\partial \phi_i} \approx \frac{f(\phi_1, \phi_2, \dots, \phi_{i-1}, \phi_i + \delta\phi_i, \phi_{i+1}, \dots, \phi_n, P, T) - f(\phi_1, \phi_2, \dots, \phi_{i-1}, \phi_i - \delta\phi_i, \phi_{i+1}, \dots, \phi_n, P, T)}{2\delta\phi_i}, \quad (3.22)$$

where $\delta\phi_i$ is a small perturbation of the molar fraction for gas component number i . Note that a new normalization of the molar fractions is needed when such a perturbation is carried out. Similarly, the partial derivatives with respect to pressure and temperature are calculated as

$$\frac{\partial f}{\partial P} \approx \frac{f(\phi_1, \phi_2, \dots, \phi_n, P + \delta P, T) - f(\phi_1, \phi_2, \dots, \phi_n, P - \delta P, T)}{2\delta P} \quad (3.23)$$

and

$$\frac{\partial f}{\partial T} \approx \frac{f(\phi_1, \phi_2, \dots, \phi_n, P, T + \delta T) - f(\phi_1, \phi_2, \dots, \phi_n, P, T - \delta T)}{2\delta T}. \quad (3.24)$$

The model uncertainty will vary depending on the actual gas parameter in question.

In this report, the combinations of gas parameters of relevance for obtaining mass flow rate, standard volume flow rate and energy flow rate in Chapters 4, 5 and 6 are listed in Table 3.1. Uncertainty of all these combinations of gas components are found by treating each of them as the parameter X and using

Eqs. (3.17), (3.21), (3.22), (3.23) and (3.24). The reason for combining them like this is that in the various functional relationships they appear in this combination.

Table 3.1 *Combination of gas parameters of relevance for the various flow meter set-ups discussed in this report.*

Type of flow meter	Type of flow rate	When densitometer is in use	When densitometer is not in use
Orifice	Mass	None	m / Z
	Standard volume	Z / Z_0	Z_0 / \sqrt{mZ}
	Energy	$H_{s,m}$	$H_{s,m} \sqrt{m / Z}$
Coriolis	Mass	Not covered in this report	None
	Standard volume		Z_0 / m
	Energy		$H_{s,m}$
Ultrasonic	Mass	None	m / Z
	Standard volume	Z / Z_0	Z / Z_0
	Energy	$H_{s,m}$	$H_{s,m} m / Z$

If, on the other hand, their uncertainties would have been treated individually, there would have been correlations between the gas parameters. These correlations would have to be treated in Chapters 4, 5 and 6. This is a complicated task that is avoided by the present approach.

In addition to these gas parameters, also the uncertainties of individual gas parameters like the CO₂ emission factors are calculated using the same type of formalism.

Of all the various individual gas parameters, it is only the compressibility factor at line conditions, Z , which depends on the line pressure and temperature. Therefore, when Z is not part of the relevant combination of gas parameters, the uncertainties of the pressure and temperature have no influence.

It is assumed that the molar mass, calorific values and CO₂ emission factors do not have any model uncertainty (more specific that such model uncertainty is negligible). However, the compressibility factors at line and standard conditions have a significant model uncertainty. The various standards (AGA 8 and ISO 6976) specify values for this model uncertainty (relative uncertainty). This means that when uncertainty of a gas parameter combination “X” listed in Table 3.1 is calculated, terms for model uncertainty must be added when the combination of gas parameters include the compressibility factor at line conditions (Z) and/or the compressibility factor at standard conditions (Z_0). The details are shown in Eqs. (3.25) - (3.31) covering all the gas parameter combinations addressed in Table 3.1:

$$\left(\frac{u((m / Z)_{\text{model}})}{m / Z} \right)^2 = \left(\frac{u(Z_{\text{model}})}{Z} \right)^2, \quad (3.25)$$

$$\left(\frac{u((Z / Z_0)_{\text{model}})}{Z / Z_0} \right)^2 = \left(\frac{u(Z_{\text{model}})}{Z} \right)^2 + \left(\frac{u(Z_{0,\text{model}})}{Z_0} \right)^2, \quad (3.26)$$

$$\left(\frac{u((Z_0 / \sqrt{mZ})_{\text{model}})}{Z_0 / \sqrt{mZ}} \right)^2 = \left(\frac{u(Z_{0,\text{model}})}{Z_0} \right)^2 + \left(\frac{1}{2} \frac{u(Z_{\text{model}})}{Z} \right)^2, \quad (3.27)$$

$$u(H_{s,m,model})^2 = 0, \quad (3.28)$$

$$\left(\frac{u\left(\left(H_{s,m} \sqrt{m/Z}\right)_{model}\right)}{H_{s,m} \sqrt{m/Z}} \right)^2 = \left(\frac{1}{2} \frac{u(Z_{model})}{Z} \right)^2, \quad (3.29)$$

$$\left(\frac{u\left(\left(Z_0 / m\right)_{model}\right)}{Z_0 / m} \right)^2 = \left(\frac{u(Z_{0,model})}{Z_0} \right)^2, \quad (3.30)$$

$$\left(\frac{u\left(\left(H_{s,m} m / Z\right)_{model}\right)}{H_{s,m} m / Z} \right)^2 = \left(\frac{u(Z_{model})}{Z} \right)^2. \quad (3.31)$$

4 Orifice fiscal metering stations

In this chapter the uncertainty models for orifice fiscal metering stations are described. The chapter is a generalization of the work in [Dahl et al, 2003], where now more set-ups of the metering station are covered.

In Section 4.1 the set-up of the orifice metering station is described. In Section 4.2 the functional relationship is described. The uncertainty models covering a single flow meter are described in Section 4.3. In Section 4.4 the uncertainty models are extended to two flow meters in parallel.

4.1 Description of metering station

The orifice metering station consists of an orifice plate with differential pressure measurement in accordance with ISO 5167:2. Furthermore, the pressure is measured upstream and the temperature is measured downstream of the orifice plate. This is in accordance with NORSOK I-106 Section 5.8, under heading "Fiscal and allocation gas systems". With respect to density and gas composition, there are three options covered:

- Density measured by downstream densitometer, gas composition used for compressibility and calorific value calculations. This gas composition can be a fixed or measured composition.
- Gas composition measured by online gas chromatograph. This composition in addition to pressure and temperature is used for calculation of density, compressibility and calorific value.
- Gas composition measured by laboratory analysis of spot gas samples. This composition in addition to pressure and temperature is used for calculation of density, compressibility and calorific value.

The orifice metering station is not flow calibrated. Discharge coefficient and expansibility coefficient are calculated according to ISO 5167:2.

When the metering station consists of two parallel pipes each equipped with orifice plate, it is assumed that each line has individual differential pressure, pressure and temperature measurement. Furthermore, if densitometers are present, each line has its own densitometer. In the case with use of gas composition, it is assumed that a common gas composition is used for both lines. This means that the same online gas chromatograph will serve both lines. Also a possible sampling point for gas samples will serve both lines.

4.2 Functional relationship

In this section, the functional relationships for mass flow rate, standard volumetric flow rate and energy flow rate are given, for a metering station with one single orifice plate (not two in parallel). Both the case with densitometer in use, and the case where density is established from gas composition (online gas chromatography or spot samples of gas analyzed in a laboratory) are covered.

4.2.1 General expressions

According to ISO 5167:2, the mass flow rate is calculated as

$$q_m = \frac{C}{\sqrt{1 - \left(\frac{d}{D}\right)^4}} \varepsilon \frac{\pi d^2}{4} \sqrt{2\rho_1 \Delta P}. \quad (4.1)$$

For definition of symbols it is referred to Appendix D. By using the equation of state, the standard volumetric flow rate can be found as

$$q_{v0} = \frac{P_1 T_0 Z_0}{P_0 T_1 Z_1} \frac{q_m}{\rho_1} = \frac{P_1 T_0 Z_0}{P_0 T_1 Z_1} \frac{C}{\sqrt{1 - \left(\frac{d}{D}\right)^4}} \varepsilon \frac{\pi d^2}{4} \sqrt{\frac{2\Delta P}{\rho_1}}. \quad (4.2)$$

Similarly, the energy flow rate can be found as

$$q_e = H_{s,m} q_m = \frac{H_{s,m} C}{\sqrt{1 - \left(\frac{d}{D}\right)^4}} \varepsilon \frac{\pi d^2}{4} \sqrt{2\rho_1 \Delta P}. \quad (4.3)$$

These three expressions will now be used to establish the functional relationship both for the case when a densitometer is in use and for the case when a densitometer is not in use.

4.2.2 Expressions when densitometer is used

In the case of a downstream densitometer, the density has to be converted from downstream to upstream conditions. With pressure measured upstream, and temperature downstream, and based on Eq. (4.1), the mass flow rate will be

$$\begin{aligned} q_m &= \frac{C}{\sqrt{1 - \left(\frac{d}{D}\right)^4}} \varepsilon \frac{\pi d^2}{4} \sqrt{2\rho_2 \frac{P_1}{(P_1 - \Delta P)} \frac{T_2}{(T_2 + \Delta T)} \frac{Z_2}{Z_1} \Delta P} \\ &= \frac{C}{\sqrt{1 - \left(\frac{d}{D}\right)^4}} \varepsilon \frac{\pi d^2}{4} \sqrt{2\rho_2 \frac{P_1}{(P_1 - \Delta P)} \frac{1}{(1 + \Delta T / T_2)} \frac{Z_2}{Z_1} \Delta P}. \end{aligned} \quad (4.4)$$

Similarly, based on Eq. (4.2), the standard volumetric flow rate will be

$$\begin{aligned} q_{v0} &= \frac{P_1 T_0 Z_0}{P_0 T_1 Z_1} \frac{C}{\sqrt{1 - \left(\frac{d}{D}\right)^4}} \varepsilon \frac{\pi d^2}{4} \sqrt{2 \frac{(P_1 - \Delta P)}{\rho_2 P_1} \frac{(T_2 + \Delta T)}{T_2} \frac{Z_1}{Z_2} \Delta P} \\ &= \frac{P_1 T_0 Z_0}{P_0 T_1 Z_1} \frac{C}{\sqrt{1 - \left(\frac{d}{D}\right)^4}} \varepsilon \frac{\pi d^2}{4} \sqrt{2 \frac{(P_1 - \Delta P)}{\rho_2 P_1} (1 + \Delta T / T_2) \frac{Z_1}{Z_2} \Delta P}. \end{aligned} \quad (4.5)$$

In addition, based on Eq.(4.3), the energy flow rate will be

$$\begin{aligned} q_e &= \frac{H_{s,m} C}{\sqrt{1 - \left(\frac{d}{D}\right)^4}} \varepsilon \frac{\pi d^2}{4} \sqrt{2\rho_2 \frac{P_1}{(P_1 - \Delta P)} \frac{T_2}{(T_2 + \Delta T)} \frac{Z_2}{Z_1} \Delta P} \\ &= \frac{H_{s,m} C}{\sqrt{1 - \left(\frac{d}{D}\right)^4}} \varepsilon \frac{\pi d^2}{4} \sqrt{2\rho_2 \frac{P_1}{(P_1 - \Delta P)} \frac{1}{(1 + \Delta T / T_2)} \frac{Z_2}{Z_1} \Delta P}. \end{aligned} \quad (4.6)$$

In the calculations carried out in the uncertainty program, for getting the relations between flow rate and differential pressure, the temperature difference over the orifice plate is neglected. This approximation will not be important for the uncertainty model and calculations carried out here.

4.2.3 Expressions when densitometer is not used

In the case when densitometer is not present, the density has to be found from the gas composition, through the equation of state. Based on Eq. (4.1), the mass flow rate will then be

$$q_m = \frac{C}{\sqrt{1 - \left(\frac{d}{D}\right)^4}} \varepsilon \frac{\pi d^2}{4} \sqrt{\frac{2P_1 m \Delta P}{Z_1 R T_1}}. \quad (4.7)$$

Similarly, based on Eq. (4.2), the standard volumetric flow rate will be

$$\begin{aligned} q_{v0} &= \frac{P_1 T_0 Z_0}{P_0 T_1 Z_1} \frac{C}{\sqrt{1 - \left(\frac{d}{D}\right)^4}} \varepsilon \frac{\pi d^2}{4} \sqrt{\frac{2Z_1 R T_1 \Delta P}{P_1 m}} \\ &= \frac{Z_0 T_0}{P_0} \frac{C}{\sqrt{1 - \left(\frac{d}{D}\right)^4}} \varepsilon \frac{\pi d^2}{4} \sqrt{\frac{2P_1 R \Delta P}{Z_1 m T_1}}. \end{aligned} \quad (4.8)$$

In addition, based on Eq.(4.3), the energy flow rate will be

$$q_e = \frac{H_{s,m} C}{\sqrt{1 - \left(\frac{d}{D}\right)^4}} \varepsilon \frac{\pi d^2}{4} \sqrt{\frac{2P_1 m \Delta P}{Z_1 R T_1}}. \quad (4.9)$$

In these formulas, the effect of thermal expansion on the two diameters, d and D , is not covered. This means that it is assumed that the effect of thermal expansion is assumed to be implemented in the flow computer. In such cases the uncertainty related to thermal expansion has earlier been shown to be negligible compared to other uncertainty contributions [Dahl et al, 2003]. In order not to make the uncertainty model more complex than necessary, it has therefore been decided to not cover thermal expansion in the uncertainty model to be described in the next sections.

4.3 Uncertainty model

In this section, the uncertainty models for the various cases described in the previous section are presented. These uncertainty models are derived from the general methodology described in the ISO GUM [ISO GUM, 2008].

4.3.1 When densitometer is used

Eq. (4.4) describes the functional relationship for the mass flow rate. By following the ISO GUM methodology, the uncertainty model for the mass flow rate can be written as

$$\begin{aligned} \left(\frac{u(q_m)}{q_m} \right)^2 = & \left(\frac{u(C)}{C} \right)^2 + \left(\frac{u(\varepsilon)}{\varepsilon} \right)^2 + \left(\frac{2(d/D)^4}{1-(d/D)^4} \right)^2 \left(\frac{u(D)}{D} \right)^2 + \left(\frac{2}{1-(d/D)^4} \right)^2 \left(\frac{u(d)}{d} \right)^2 \\ & + \left(\frac{1}{2} \right)^2 \left(\frac{u(\rho_2)}{\rho_2} \right)^2 + \left(\frac{1}{2} \frac{P_1}{P_1 - \Delta P} \right)^2 \left(\frac{u(\Delta P)}{\Delta P} \right)^2 + \left(\frac{1}{2} \frac{\Delta P}{P_1 - \Delta P} \right)^2 \left(\frac{u(P_1)}{P_1} \right)^2. \end{aligned} \quad (4.10)$$

Eq. (4.5) describes the functional relationship for the standard volumetric flow rate. The compressibility factors at standard and line conditions depend both on the gas composition, and in order to avoid correlations, their uncertainties are treated together in the uncertainty model. By following the ISO GUM methodology, the uncertainty model for the standard volumetric flow rate can be written as

$$\begin{aligned} \left(\frac{u(q_{v0})}{q_{v0}} \right)^2 = & \left(\frac{2P_1 - \Delta P}{2P_1 - 2\Delta P} \right)^2 \left(\frac{u(P_1)}{P_1} \right)^2 + \left(\frac{u(T_1)}{T_1} \right)^2 + \left(\frac{u(Z_1/Z_0)}{Z_1/Z_0} \right)^2 + \left(\frac{u(C)}{C} \right)^2 + \left(\frac{u(\varepsilon)}{\varepsilon} \right)^2 \\ & + \left(\frac{2(d/D)^4}{1-(d/D)^4} \right)^2 \left(\frac{u(D)}{D} \right)^2 + \left(\frac{2}{1-(d/D)^4} \right)^2 \left(\frac{u(d)}{d} \right)^2 + \left(\frac{1}{2} \right)^2 \left(\frac{u(\rho_2)}{\rho_2} \right)^2 \\ & + \left(\frac{P_1 - 2\Delta P}{2P_1 - 2\Delta P} \right)^2 \left(\frac{u(\Delta P)}{\Delta P} \right)^2. \end{aligned} \quad (4.11)$$

Eq. (4.6) describes the functional relationship for the energy flow rate. By following the ISO GUM methodology, the uncertainty model for the energy flow rate can be written as

$$\begin{aligned} \left(\frac{u(q_e)}{q_e} \right)^2 = & \left(\frac{u(H_{s,m})}{H_{s,m}} \right)^2 + \left(\frac{u(C)}{C} \right)^2 + \left(\frac{u(\varepsilon)}{\varepsilon} \right)^2 \\ & + \left(\frac{2(d/D)^4}{1-(d/D)^4} \right)^2 \left(\frac{u(D)}{D} \right)^2 + \left(\frac{2}{1-(d/D)^4} \right)^2 \left(\frac{u(d)}{d} \right)^2 \\ & + \left(\frac{1}{2} \right)^2 \left(\frac{u(\rho_2)}{\rho_2} \right)^2 + \left(\frac{1}{2} \frac{P_1}{P_1 - \Delta P} \right)^2 \left(\frac{u(\Delta P)}{\Delta P} \right)^2 + \left(\frac{1}{2} \frac{\Delta P}{P_1 - \Delta P} \right)^2 \left(\frac{u(P_1)}{P_1} \right)^2. \end{aligned} \quad (4.12)$$

4.3.2 When densitometer is not used

Eq. (4.7) describes the functional relationship for the mass flow rate. The molar mass and the compressibility factor at line conditions depend both on the gas composition, and in order to avoid correlations, their uncertainties are treated together in the uncertainty model. By following the ISO GUM methodology, the uncertainty model for the mass flow rate can be written as

$$\begin{aligned} \left(\frac{u(q_m)}{q_m} \right)^2 = & \left(\frac{u(C)}{C} \right)^2 + \left(\frac{u(\varepsilon)}{\varepsilon} \right)^2 + \left(\frac{2(d/D)^4}{1-(d/D)^4} \right)^2 \left(\frac{u(D)}{D} \right)^2 + \left(\frac{2}{1-(d/D)^4} \right)^2 \left(\frac{u(d)}{d} \right)^2 \\ & + \left(\frac{1}{2} \right)^2 \left(\frac{u(\Delta P)}{\Delta P} \right)^2 + \left(\frac{1}{2} \right)^2 \left(\frac{u(P_1)}{P_1} \right)^2 + \left(\frac{1}{2} \right)^2 \left(\frac{u(m/Z_1)}{m/Z_1} \right)^2 + \left(\frac{1}{2} \right)^2 \left(\frac{u(T_1)}{T_1} \right)^2. \end{aligned} \quad (4.13)$$

Eq. (4.8) describes the functional relationship for the standard volume flow rate. The molar mass and the compressibility factors at standard and line conditions depend all on the gas composition, and in order to avoid correlations, their uncertainties are treated together in the uncertainty model. By following the ISO GUM methodology, the uncertainty model for the standard volumetric flow rate can be written as

$$\begin{aligned} \left(\frac{u(q_{v0})}{q_{v0}} \right)^2 = & \left(\frac{u(C)}{C} \right)^2 + \left(\frac{u(\varepsilon)}{\varepsilon} \right)^2 + \left(\frac{2(d/D)^4}{1-(d/D)^4} \right)^2 \left(\frac{u(D)}{D} \right)^2 + \left(\frac{2}{1-(d/D)^4} \right)^2 \left(\frac{u(d)}{d} \right)^2 \\ & + \left(\frac{1}{2} \right)^2 \left(\frac{u(\Delta P)}{\Delta P} \right)^2 + \left(\frac{1}{2} \right)^2 \left(\frac{u(P_1)}{P_1} \right)^2 + \left(\frac{u(Z_0/\sqrt{mZ_1})}{Z_0/\sqrt{mZ_1}} \right)^2 + \left(\frac{1}{2} \right)^2 \left(\frac{u(T_1)}{T_1} \right)^2. \end{aligned} \quad (4.14)$$

Eq. (4.9) describes the functional relationship for the energy flow rate. The calorific value, molar mass and the compressibility factor at line conditions depend all on the gas composition, and in order to avoid correlations, their uncertainties are treated together in the uncertainty model. By following the ISO GUM methodology, the uncertainty model for the energy flow rate then can be written as

$$\begin{aligned} \left(\frac{u(q_e)}{q_e} \right)^2 = & \left(\frac{u(C)}{C} \right)^2 + \left(\frac{u(\varepsilon)}{\varepsilon} \right)^2 + \left(\frac{2(d/D)^4}{1-(d/D)^4} \right)^2 \left(\frac{u(D)}{D} \right)^2 + \left(\frac{2}{1-(d/D)^4} \right)^2 \left(\frac{u(d)}{d} \right)^2 \\ & + \left(\frac{1}{2} \right)^2 \left(\frac{u(\Delta P)}{\Delta P} \right)^2 + \left(\frac{1}{2} \right)^2 \left(\frac{u(P_1)}{P_1} \right)^2 + \left(\frac{u(H_{s,m}\sqrt{m/Z_1})}{H_{s,m}\sqrt{m/Z_1}} \right)^2 + \left(\frac{1}{2} \right)^2 \left(\frac{u(T_1)}{T_1} \right)^2. \end{aligned} \quad (4.15)$$

4.4 Two flow meters in parallel

4.4.1 Correlation classification

The generic uncertainty model for two flow meters in parallel is given in Appendix B. The uncertainty model is developed under the assumption that the flow rate is about the same in both pipes.

Based on the results of the uncertainty model development in Appendix B, it is necessary to classify all uncertainty contributions as either correlated or uncorrelated between the two flow meters. The following assumptions and evaluations have been made in order to classify the correlations:

- **Discharge coefficient:** This uncertainty is assumed to be **uncorrelated** between pipe A and B. This coefficient is related to the flow profile thus the inlet pipe work to the metering station. This will never be identical in the two pipes.
- **Expansibility factor:** This uncertainty is assumed to be **uncorrelated** between pipe A and B. The uncertainty in this factor is partly due to the flow profile and partly to the gas properties. There are good reasons both for classifying the uncertainty as correlated and uncorrelated. However, as this usually is a negligible uncertainty contribution, a brief classification as uncorrelated can be made.
- **Pipe diameter:** This uncertainty is assumed to be **correlated**. This is because it is expected that the pipe work in the two pipes is delivered from the same vendor and produced under the same batch. Therefore, correlations can be expected.
- **Orifice diameter:** This uncertainty is assumed to be **correlated**. This is because it is expected that the orifice plates in the two pipes are delivered from the same vendor and dimensions are

measured at the same time and using the same equipment. Therefore, correlations can be expected.

- **Differential pressure:** This uncertainty is assumed to be **uncorrelated**. This is because two different differential pressure instruments are used. Even if they are of the same type, they may not be calibrated at the same time. It is therefore expected that the uncertainty mainly is uncorrelated.
- **Measured density:** This uncertainty is assumed to be **uncorrelated**. This is because two different densitometers are used (one in each run). Even if they are of the same type, they may not be calibrated at the same time. It is therefore expected that the uncertainty mainly is uncorrelated.
- **Pressure:** This uncertainty is assumed to be **uncorrelated**. This is because different pressure instruments are used in each run. Even if they are of the same type, they may not be calibrated at the same time. It is therefore expected that the uncertainty mainly is uncorrelated.
- **Temperature:** This uncertainty is assumed to be **uncorrelated**. This is because different temperature instruments are used. Even if they are of the same type, they may not be calibrated at the same time. It is therefore expected that the uncertainty mainly is uncorrelated.
- **Gas quality parameters:** This uncertainty is assumed to be **correlated**. It covers compressibility, molar mass and calorific value, either isolated or combined through products, ratios and powers. It is assumed that there will be a common gas chromatograph for both lines (not individual gas chromatograph for each line). Therefore, the calculation of these gas parameters is based on the same gas composition in each pipe. Therefore correlations have to be expected. In the case of gas composition based on gas sampling it is assumed a common sampling point for the two lines. Therefore, also in this case correlations have to be expected.

4.4.2 Specific uncertainty models, when densitometer is in use

Based on the uncertainty models for one orifice metering station (mass flow rate Eq. (4.10), standard volume flow rate Eq. (4.11) and energy flow rate Eq. (4.12)), the general model for combining these uncertainty models into a model for two in parallel (Section B 2) and the classification of uncertainty contributions as either correlated or uncorrelated, the uncertainty models for two flow meters in parallel can be found.

The uncertainty model for the total mass flow rate of two orifice flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned}
 \left(\frac{u(q_m)}{q_m} \right)^2 = & \frac{1}{4} \left\{ \left(\frac{u(C_A)}{C_A} \right)^2 + \left(\frac{u(C_B)}{C_B} \right)^2 + \left(\frac{u(\varepsilon_A)}{\varepsilon_A} \right)^2 + \left(\frac{u(\varepsilon_B)}{\varepsilon_B} \right)^2 \right. \\
 & + \left(\left(\frac{2(d_A/D_A)^4}{1-(d_A/D_A)^4} \right) \left(\frac{u(D_A)}{D_A} \right) + \left(\frac{2(d_B/D_B)^4}{1-(d_B/D_B)^4} \right) \left(\frac{u(D_B)}{D_B} \right) \right)^2 \\
 & + \left(\left(\frac{2}{1-(d_A/D_A)^4} \right) \left(\frac{u(d_A)}{d_A} \right) + \left(\frac{2}{1-(d_B/D_B)^4} \right) \left(\frac{u(d_B)}{d_B} \right) \right)^2 \\
 & + \left(\frac{1}{2} \right)^2 \left(\frac{u(\rho_{2A})}{\rho_{2A}} \right)^2 + \left(\frac{1}{2} \right)^2 \left(\frac{u(\rho_{2B})}{\rho_{2B}} \right)^2 \\
 & + \left(\frac{1}{2} \frac{P_{1A}}{P_{1A} - \Delta P_A} \right)^2 \left(\frac{u(\Delta P_A)}{\Delta P_A} \right)^2 + \left(\frac{1}{2} \frac{P_{1B}}{P_{1B} - \Delta P_B} \right)^2 \left(\frac{u(\Delta P_B)}{\Delta P_B} \right)^2 \\
 & \left. + \left(\frac{1}{2} \frac{\Delta P_A}{P_{1A} - \Delta P_A} \right)^2 \left(\frac{u(P_{1A})}{P_{1A}} \right)^2 + \left(\frac{1}{2} \frac{\Delta P_B}{P_{1B} - \Delta P_B} \right)^2 \left(\frac{u(P_{1B})}{P_{1B}} \right)^2 \right\}.
 \end{aligned} \tag{4.16}$$

The uncertainty model for the total standard volume flow rate of two orifice flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned}
 \left(\frac{u(q_{v0})}{q_{v0}} \right)^2 = & \frac{1}{4} \left\{ \left(\frac{2P_{1A} - \Delta P_A}{2P_{1A} - 2\Delta P_A} \right)^2 \left(\frac{u(P_{1A})}{P_{1A}} \right)^2 + \left(\frac{2P_{1B} - \Delta P_B}{2P_{1B} - 2\Delta P_B} \right)^2 \left(\frac{u(P_{1B})}{P_{1B}} \right)^2 \right. \\
 & + \left(\frac{u(T_{1A})}{T_{1A}} \right)^2 + \left(\frac{u(T_{1B})}{T_{1B}} \right)^2 + \left(\frac{u(Z_{1A}/Z_{0A})}{Z_{1A}/Z_{0A}} + \frac{u(Z_{1B}/Z_{0B})}{Z_{1B}/Z_{0B}} \right)^2 \\
 & + \left(\frac{u(C_A)}{C_A} \right)^2 + \left(\frac{u(C_B)}{C_B} \right)^2 + \left(\frac{u(\varepsilon_A)}{\varepsilon_A} \right)^2 + \left(\frac{u(\varepsilon_B)}{\varepsilon_B} \right)^2 \\
 & + \left(\left(\frac{2(d_A/D_A)^4}{1-(d_A/D_A)^4} \right) \left(\frac{u(D_A)}{D_A} \right) + \left(\frac{2(d_B/D_B)^4}{1-(d_B/D_B)^4} \right) \left(\frac{u(D_B)}{D_B} \right) \right)^2 \\
 & + \left(\left(\frac{2}{1-(d_A/D_A)^4} \right) \left(\frac{u(d_A)}{d_A} \right) + \left(\frac{2}{1-(d_B/D_B)^4} \right) \left(\frac{u(d_B)}{d_B} \right) \right)^2 \\
 & + \left(\frac{1}{2} \right)^2 \left(\frac{u(\rho_{2A})}{\rho_{2A}} \right)^2 + \left(\frac{1}{2} \right)^2 \left(\frac{u(\rho_{2B})}{\rho_{2B}} \right)^2 \\
 & \left. + \left(\frac{P_{1A} - 2\Delta P_A}{2P_{1A} - 2\Delta P_A} \right)^2 \left(\frac{u(\Delta P_A)}{\Delta P_A} \right)^2 + \left(\frac{P_{1B} - 2\Delta P_B}{2P_{1B} - 2\Delta P_B} \right)^2 \left(\frac{u(\Delta P_B)}{\Delta P_B} \right)^2 \right\}.
 \end{aligned} \tag{4.17}$$

The uncertainty model for the total energy flow rate of two orifice flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned}
\left(\frac{u(q_e)}{q_e}\right)^2 = & \frac{1}{4} \left\{ \left(\frac{u(H_{s,mA})}{H_{s,mA}} + \frac{u(H_{s,mB})}{H_{s,mB}} \right)^2 \right. \\
& + \left(\frac{u(C_A)}{C_A} \right)^2 + \left(\frac{u(C_B)}{C_B} \right)^2 + \left(\frac{u(\varepsilon_A)}{\varepsilon_A} \right)^2 + \left(\frac{u(\varepsilon_B)}{\varepsilon_B} \right)^2 \\
& + \left(\left(\frac{2(d_A/D_A)^4}{1-(d_A/D_A)^4} \right) \left(\frac{u(D_A)}{D_A} \right) + \left(\frac{2(d_B/D_B)^4}{1-(d_B/D_B)^4} \right) \left(\frac{u(D_B)}{D_B} \right) \right)^2 \\
& + \left(\left(\frac{2}{1-(d_A/D_A)^4} \right) \left(\frac{u(d_A)}{d_A} \right) + \left(\frac{2}{1-(d_B/D_B)^4} \right) \left(\frac{u(d_B)}{d_B} \right) \right)^2 \\
& + \left(\frac{1}{2} \right)^2 \left(\frac{u(\rho_{2A})}{\rho_{2A}} \right)^2 + \left(\frac{1}{2} \right)^2 \left(\frac{u(\rho_{2B})}{\rho_{2AB}} \right)^2 \\
& + \left(\frac{1}{2} \frac{P_{1A}}{P_{1A} - \Delta P_A} \right)^2 \left(\frac{u(\Delta P_A)}{\Delta P_A} \right)^2 + \left(\frac{1}{2} \frac{P_{1B}}{P_{1B} - \Delta P_B} \right)^2 \left(\frac{u(\Delta P_B)}{\Delta P_B} \right)^2 \\
& \left. + \left(\frac{1}{2} \frac{\Delta P_A}{P_{1A} - \Delta P_A} \right)^2 \left(\frac{u(P_{1A})}{P_{1A}} \right)^2 + \left(\frac{1}{2} \frac{\Delta P_B}{P_{1B} - \Delta P_B} \right)^2 \left(\frac{u(P_{1B})}{P_{1B}} \right)^2 \right\}.
\end{aligned} \tag{4.18}$$

4.4.3 Specific uncertainty models, when densitometer is not in use

Based on the uncertainty models for one orifice metering station (mass flow rate Eq. (4.13), standard volume flow rate Eq. (4.14) and energy flow rate Eq. (4.15)), the general model for combining these uncertainty models into a model for two in parallel (Section B 2) and the classification of uncertainty contributions as either correlated or uncorrelated, the uncertainty models for two flow meters in parallel can be found.

The uncertainty model for the total mass flow rate of two orifice flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned}
 \left(\frac{u(q_m)}{q_m} \right)^2 = & \frac{1}{4} \left\{ \left(\frac{u(C_A)}{C_A} \right)^2 + \left(\frac{u(C_B)}{C_B} \right)^2 + \left(\frac{u(\varepsilon_A)}{\varepsilon_A} \right)^2 + \left(\frac{u(\varepsilon_B)}{\varepsilon_B} \right)^2 + \right. \\
 & \left(\left(\frac{2(d_A/D_A)^4}{1-(d_A/D_A)^4} \right) \left(\frac{u(D_A)}{D_A} \right) + \left(\frac{2(d_B/D_B)^4}{1-(d_B/D_B)^4} \right) \left(\frac{u(D_B)}{D_B} \right) \right)^2 \\
 & + \left(\left(\frac{2}{1-(d_A/D_A)^4} \right) \left(\frac{u(d_A)}{d_A} \right) + \left(\frac{2}{1-(d_B/D_B)^4} \right) \left(\frac{u(d_B)}{d_B} \right) \right)^2 \\
 & + \left(\frac{1}{2} \right)^2 \left(\frac{u(\Delta P_A)}{\Delta P_A} \right)^2 + \left(\frac{1}{2} \right)^2 \left(\frac{u(\Delta P_B)}{\Delta P_B} \right)^2 \\
 & + \left(\frac{1}{2} \right)^2 \left(\frac{u(P_{1A})}{P_{1A}} \right)^2 + \left(\frac{1}{2} \right)^2 \left(\frac{u(P_{1B})}{P_{1B}} \right)^2 \\
 & + \left(\left(\frac{1}{2} \right) \left(\frac{u(m_A/Z_{1A})}{m_A/Z_{1A}} \right) + \left(\frac{1}{2} \right) \left(\frac{u(m_B/Z_{1B})}{m_B/Z_{1B}} \right) \right)^2 \\
 & \left. + \left(\frac{1}{2} \right)^2 \left(\frac{u(T_{1A})}{T_{1A}} \right)^2 + \left(\frac{1}{2} \right)^2 \left(\frac{u(T_{1B})}{T_{1B}} \right)^2 \right\}.
 \end{aligned} \tag{4.19}$$

The uncertainty model for the total standard volume flow rate of two orifice flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned}
\left(\frac{u(q_{v0})}{q_{v0}}\right)^2 = & \frac{1}{4} \left\{ \left(\frac{u(C_A)}{C_A}\right)^2 + \left(\frac{u(C_B)}{C_B}\right)^2 + \left(\frac{u(\varepsilon_A)}{\varepsilon_A}\right)^2 + \left(\frac{u(\varepsilon_B)}{\varepsilon_B}\right)^2 + \right. \\
& \left(\left(\frac{2(d_A/D_A)^4}{1-(d_A/D_A)^4}\right) \left(\frac{u(D_A)}{D_A}\right) + \left(\frac{2(d_B/D_B)^4}{1-(d_B/D_B)^4}\right) \left(\frac{u(D_B)}{D_B}\right) \right)^2 \\
& + \left(\left(\frac{2}{1-(d_A/D_A)^4}\right) \left(\frac{u(d_A)}{d_A}\right) + \left(\frac{2}{1-(d_B/D_B)^4}\right) \left(\frac{u(d_B)}{d_B}\right) \right)^2 \\
& + \left(\frac{1}{2}\right)^2 \left(\frac{u(\Delta P_A)}{\Delta P_A}\right)^2 + \left(\frac{1}{2}\right)^2 \left(\frac{u(\Delta P_B)}{\Delta P_B}\right)^2 \\
& + \left(\frac{1}{2}\right)^2 \left(\frac{u(P_{1A})}{P_{1A}}\right)^2 + \left(\frac{1}{2}\right)^2 \left(\frac{u(P_{1B})}{P_{1B}}\right)^2 \\
& + \left(\left(\frac{u(Z_{0A}/\sqrt{m_A Z_{1A}})}{Z_{0A}/\sqrt{m_A Z_{1A}}}\right) + \left(\frac{u(Z_{0B}/\sqrt{m_B Z_{1B}})}{Z_{0B}/\sqrt{m_B Z_{1B}}}\right) \right)^2 \\
& \left. + \left(\frac{1}{2}\right)^2 \left(\frac{u(T_{1A})}{T_{1A}}\right)^2 + \left(\frac{1}{2}\right)^2 \left(\frac{u(T_{1B})}{T_{1B}}\right)^2 \right\}.
\end{aligned} \tag{4.20}$$

The uncertainty model for the total energy flow rate of two orifice flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned}
\left(\frac{u(q_e)}{q_e}\right)^2 = & \frac{1}{4} \left\{ \left(\frac{u(C_A)}{C_A}\right)^2 + \left(\frac{u(C_B)}{C_B}\right)^2 + \left(\frac{u(\varepsilon_A)}{\varepsilon_A}\right)^2 + \left(\frac{u(\varepsilon_B)}{\varepsilon_B}\right)^2 + \right. \\
& \left(\left(\frac{2(d_A/D_A)^4}{1-(d_A/D_A)^4}\right) \left(\frac{u(D_A)}{D_A}\right) + \left(\frac{2(d_B/D_B)^4}{1-(d_B/D_B)^4}\right) \left(\frac{u(D_B)}{D_B}\right) \right)^2 \\
& + \left(\left(\frac{2}{1-(d_A/D_A)^4}\right) \left(\frac{u(d_A)}{d_A}\right) + \left(\frac{2}{1-(d_B/D_B)^4}\right) \left(\frac{u(d_B)}{d_B}\right) \right)^2 \\
& + \left(\frac{1}{2}\right)^2 \left(\frac{u(\Delta P_A)}{\Delta P_A}\right)^2 + \left(\frac{1}{2}\right)^2 \left(\frac{u(\Delta P_B)}{\Delta P_B}\right)^2 \\
& + \left(\frac{1}{2}\right)^2 \left(\frac{u(P_{1A})}{P_{1A}}\right)^2 + \left(\frac{1}{2}\right)^2 \left(\frac{u(P_{1B})}{P_{1B}}\right)^2 \\
& + \left(\left(\frac{u(H_{s,mA}\sqrt{m_A/Z_{1A}})}{H_{s,mA}\sqrt{m_A/Z_{1A}}}\right) + \left(\frac{u(H_{s,mB}\sqrt{m_B/Z_{1B}})}{H_{s,mB}\sqrt{m_B/Z_{1B}}}\right) \right)^2 \\
& \left. + \left(\frac{1}{2}\right)^2 \left(\frac{u(T_{1A})}{T_{1A}}\right)^2 + \left(\frac{1}{2}\right)^2 \left(\frac{u(T_{1B})}{T_{1B}}\right)^2 \right\}.
\end{aligned} \tag{4.21}$$

5 Coriolis fiscal metering station

In this chapter, uncertainty models for mass flow rate, standard volume flow rate and energy flow rate for a Coriolis flow metering station are presented. In Section 5.1 the set-up of the metering station is given. In Section 5.2 the functional relationship for the mass flow rate, standard volume flow rate and energy flow rate for a metering station with one Coriolis flow meter is presented. Section 5.3 gives the uncertainty model for the mass flow rate for a single Coriolis flow meter. In Section 5.4 this is extended to uncertainty models also for standard volume flow rate and energy flow rate. Section 5.5 gives the uncertainty model for the total flow rates from two Coriolis flow meters in parallel, and Section 5.6 for the average flow rates from two Coriolis flow meters in series.

5.1 Description of metering station

The Coriolis metering station consists of a Coriolis mass flow meter in accordance with ISO 10790. In addition, pressure and temperature is measured. It is assumed that density, compressibility and calorific value are calculated based on a gas composition. There are three options covered:

- A given, fixed composition.
- Gas composition measured by online gas chromatograph.
- Gas composition measured by laboratory analysis of spot gas samples.

In addition the cases of two flow meters in parallel and two flow meters in series are covered. It is assumed that the same gas composition is used for both flow meters

5.2 Functional relationship

5.2.1 Mass flow rate, flow calibrated Coriolis meter

The Coriolis flow meter measures the mass flow rate as its primary output. Typically, the Coriolis flow meter will be flow calibrated. Thus, an adjustment of the flow meter may be carried out.

The flow calibration is carried by comparing the mass flow rate output from the Coriolis flow meter with the similar reading from a reference measurement. This is carried out at a set of N different flow rates.

The details are covered in Appendix A, where “ x ” is replaced by “ m ” and “*Meter*” is replaced by “*Coriolis*” in the index of the flow rate q in the formulas. Three different ways of correcting the flow meter are covered:

- (i) no correction,
- (ii) a constant percentage correction,
- (iii) linear interpolation.

Appendix A describes the percentage deviation that is corrected (“ p ”) in all these three cases, and how this is converted to a correction factor K .

It should, however, be commented that the third case (linear interpolation) provides a correction such that the flow meter’s flow rate will be corrected to the reference meter flow rate, when the flow rate is equal to any of the flow rates used in the flow calibration. This case is therefore in agreement with the

Norwegian Petroleum Directorate Measurement Regulations [NPD], where one requirement in Section 8 is that “*The measurement system shall be designed so that systematic measurement errors are avoided or compensated for*”. Using case (i) and (ii) is not in agreement with this requirement.

5.2.2 Standard volumetric flow rate and energy flow rate, flow calibrated Coriolis meter

In the previous subsection it is described how the mass flow rate from a flow calibrated Coriolis flow meter is found. The standard volumetric flow rate can now be found by using a gas composition coming from either an online gas chromatograph, from spot sampling, or from a fixed composition. In all three cases, the standard volumetric flow rate can be written as

$$q_{v0} = \frac{Z_0 R T_0}{m P_0} q_m. \quad (5.1)$$

Similarly, the energy flow rate can be found as

$$q_e = H_{s,m} q_m. \quad (5.2)$$

5.3 Uncertainty model, mass flow rate

The uncertainty of the mass flow rate of a flow calibrated Coriolis meter consists of two general uncertainty contributions

- Calibration uncertainty
- Field uncertainty

Formally, this can be written as

$$\left(\frac{u(q_m)}{q_m} \right)^2 = \left(\frac{u(q_{m,cal})}{q_m} \right)^2 + \left(\frac{u(q_{m,field})}{q_m} \right)^2. \quad (5.3)$$

These two contributions will now be discussed more in detail.

5.3.1 Calibration uncertainty

The calibration uncertainty consists of the following three contributions:

- Uncertainty of the correction factor estimate (the adjustment after deviations between flow meter and reference measurement at the flow laboratory are established).
- Uncertainty of the reference measurement at the flow laboratory.
- Repeatability, including both the Coriolis flow meter to be calibrated and the reference measurement.

This can be written as

$$\left(\frac{u(q_{m,cal})}{q_m} \right)^2 = \left(\frac{u(q_{m,cal,dev})}{q_m} \right)^2 + \left(\frac{u(q_{m,cal,ref})}{q_m} \right)^2 + \left(\frac{u(q_{m,cal,rept})}{q_m} \right)^2. \quad (5.4)$$

These three terms will now be discussed more in detail.

Uncertainty of the correction factor estimate: This uncertainty contribution is described in Appendix A, where, where “x” is replaced by “m” and “Meter” is replaced by “Coriolis” in the index of the flow rate q in the formulas. It is calculated from the deviation between the Coriolis flow meter mass flow rate and the mass flow rate measured by the reference meter, at a series of mass flow rates. Three adjustment methods for the Coriolis flow meter are discussed:

- (i) no correction,
- (ii) a constant percentage correction,
- (iii) linear interpolation.

For each of these methods, the actual expression is given in Appendix A for any uncorrected percentage deviation, δp , of the flow meter after adjustment of the Coriolis flow meter.

As described in Appendix A, the relative standard uncertainty of the correction factor estimate can be written as

$$\left(\frac{u(q_{m,cal,dev})}{q_m} \right) = \left(\frac{u(K)}{K} \right) = \frac{1}{K} \frac{\partial p}{\partial K} u(p) = \frac{\delta p / \sqrt{3}}{100 + p}. \quad (5.5)$$

Uncertainty of the reference measurement: This term depends on the metering equipment at the flow laboratory. This number is usually found in the calibration certificate. It can depend on the flow rate. Therefore, for mass flow rates between the ones used in the flow calibration, a linear interpolation based on the values of this uncertainty at the mass flow rates used in flow calibration is used. The relative uncertainty at the highest calibrated flow rate will be used for flow rates above this highest calibrated flow rate. The relative uncertainty at the lowest calibrated flow rate will be used for flow rates below this lowest calibrated flow rate.

Repeatability: This term covers both the repeatability of the Coriolis flow meter to be calibrated and the reference measurement. It can vary with mass flow rate. Therefore, for mass flow rates between the ones used in the flow calibration, a linear interpolation based on the values of this repeatability at the mass flow rates used in flow calibration is used. The repeatability at the highest calibrated flow rate will be used for flow rates above this highest calibrated flow rate. The repeatability at the lowest calibrated flow rate will be used for flow rates below this lowest calibrated flow rate.

5.3.2 Field uncertainty

The field uncertainty will consist of the following two contributions

- Repeatability of the flow meter under field operation
- Uncertainty due to changes of conditions from flow calibration to field operation

This can be written as

$$\left(\frac{u(q_{m,field})}{q_m} \right)^2 = \left(\frac{u(q_{m,field,rept})}{q_m} \right)^2 + \left(\frac{u(q_{m,field,cond})}{q_m} \right)^2. \quad (5.6)$$

These two terms will now be discussed more in detail.

Repeatability of the flow meter under field operation: This can usually be found in the data sheet of the flow meter, if not own experience is used for establishing the repeatability. It is possible to specify different values on the repeatability for different flow rates. In that case linear interpolation is used for obtaining the repeatability at mass flow rates in-between the ones where the repeatability is specified. The repeatability at the highest calibrated flow rate will be used for flow rates above this highest calibrated flow rate. The repeatability at the lowest calibrated flow rate will be used for flow rates below this lowest calibrated flow rate.

Uncertainty due to changes of conditions from flow calibration to field operation: The value of this quantity will depend on the actual installation and on the data sheet of the flow meter. It is possible to specify different values on the relative uncertainty at different flow rates. In that case linear interpolation is used for obtaining the relative uncertainty at mass flow rates in-between the ones where it is specified. The relative uncertainty at the highest calibrated flow rate will be used for flow rates above this highest calibrated flow rate. The relative uncertainty at the lowest calibrated flow rate will be used for flow rates below this lowest calibrated flow rate.

5.3.3 Total uncertainty in mass flow rate, one flow meter

Based on the two previous sub-sections, the total uncertainty model for the mass flow rate from a flow calibrated Coriolis flow meter can be written as

$$\begin{aligned} \left(\frac{u(q_m)}{q_m} \right)^2 = & \left(\frac{u(q_{m,cal,dev})}{q_m} \right)^2 + \left(\frac{u(q_{m,cal,ref})}{q_m} \right)^2 + \left(\frac{u(q_{m,cal,rept})}{q_m} \right)^2 \\ & + \left(\frac{u(q_{m,field,rept})}{q_m} \right)^2 + \left(\frac{u(q_{m,field,cond})}{q_m} \right)^2. \end{aligned} \quad (5.7)$$

5.4 Uncertainty model, standard volume and energy flow rate

Eq. (5.1) describes the functional relationship between the mass flow rate and the standard volumetric flow rate. The molar mass and the compressibility factor at standard conditions depend both on the gas composition, and in order to avoid correlations, the uncertainty model for the standard volumetric flow rate is written as

$$\left(\frac{u(q_{v0})}{q_{v0}} \right)^2 = \left(\frac{u(q_m)}{q_m} \right)^2 + \left(\frac{u(Z_0/m)}{Z_0/m} \right)^2. \quad (5.8)$$

Eq. (5.2) describes the functional relationship between the mass flow rate and the energy flow rate. The mass based superior calorific value depends on the gas composition, and has thus uncertainty. The uncertainty model for the energy flow rate is written as

$$\left(\frac{u(q_e)}{q_e} \right)^2 = \left(\frac{u(q_m)}{q_m} \right)^2 + \left(\frac{u(H_{s,m})}{H_{s,m}} \right)^2. \quad (5.9)$$

5.5 Two flow meters in parallel

5.5.1 Correlation classification

The generic uncertainty model for two flow meters in parallel is given in Appendix B. The uncertainty model is developed under the assumption that the flow rate is about the same in both pipes.

Based on the results of the uncertainty model development in Appendix B, it is necessary to classify all uncertainty contributions as either correlated or uncorrelated between the two flow meters. The following assumptions and evaluations have been made in order to classify the correlations:

- **Calibration uncertainty**
 - *Uncertainty of the correction factor estimate (the adjustment after deviations between flow meter and reference measurement at the flow laboratory are established):* It is assumed that this uncertainty contribution is **uncorrelated** as each meter will have its own deviation curve, and possible errors due to linear interpolation in such a deviation curve are not likely to repeat between different meters.
 - *Uncertainty of the reference measurement at the flow laboratory:* If the two flow meters are calibrated at the same time at the same location, it is likely that this uncertainty contribution is **correlated**, as the flow meters are compared to the same reference. In other cases it is likely that it is **uncorrelated**. In the uncertainty program it is possible to specify whether the flow meters are calibrated at the same time and location or not.
 - *Repeatability, including both the Coriolis flow meter to be calibrated and the reference measurement:* This represents random variations, and will thus be **uncorrelated** between the two flow meters.
- **Field uncertainty**
 - *Repeatability of the flow meter under field operation:* this represents random variations, and will thus be **uncorrelated** between the two flow meters.
 - *Uncertainty due to changes of conditions from flow calibration to field operation:* It is here assumed that this is **uncorrelated**. This is because the flow conditions will never be identical in two different pipes, and therefore it is likely that they may be affected differently by changed conditions from calibration to field.
- **Gas parameters**
 - *The uncertainty of the fraction of standard compressibility to molar mass* is used in the uncertainty model for standard volume flow rate. As it is assumed that the same gas composition is used for both flow meters, this parameter is **correlated**.
 - *The uncertainty of the mass based superior calorific value* is used in the uncertainty model for energy flow rate. As it is assumed that the same gas composition is used for both flow meters, this parameter is **correlated**.

5.5.2 Specific uncertainty models

Based on the uncertainty models for one flow calibrated Coriolis meter (mass flow rate Eq. (5.7), standard volume flow rate Eq. (5.8) and energy flow rate Eq. (5.9)), the general model for combining these uncertainty models into a model for two in parallel (Section B 2) and the classification of uncertainty contributions as either correlated or uncorrelated, the uncertainty models for two flow meters in parallel can be found.

If the two flow meters are calibrated at the same time and location:

The uncertainty model for the total mass flow rate of two flow calibrated Coriolis flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned}
\left(\frac{u(q_m)}{q_m}\right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{m,cal,devA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,devB})}{q_{mB}}\right)^2 + \left(\frac{u(q_{m,cal,refA})}{q_{mA}} + \frac{u(q_{m,cal,refB})}{q_{mB}}\right)^2 \right. \\
& + \left(\frac{u(q_{m,cal,repA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,repB})}{q_{mB}}\right)^2 + \left(\frac{u(q_{m,field,repA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,field,repB})}{q_{mB}}\right)^2 \\
& \left. + \left(\frac{u(q_{m,field,condA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,field,condB})}{q_{mB}}\right)^2 \right\}. \quad (5.10)
\end{aligned}$$

The uncertainty model for the total standard volume flow rate of two flow calibrated Coriolis flow meters in parallel can be written as

$$\begin{aligned}
\left(\frac{u(q_{v0})}{q_{v0}}\right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{m,cal,devA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,devB})}{q_{mB}}\right)^2 + \left(\frac{u(q_{m,cal,refA})}{q_{mA}} + \frac{u(q_{m,cal,refB})}{q_{mB}}\right)^2 \right. \\
& + \left(\frac{u(q_{m,cal,repA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,repB})}{q_{mB}}\right)^2 + \left(\frac{u(q_{m,field,repA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,field,repB})}{q_{mB}}\right)^2 \\
& \left. + \left(\frac{u(q_{m,field,condA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,field,condB})}{q_{mB}}\right)^2 + \left(\frac{u(Z_{0A}/m_A)}{Z_{0A}/m_A} + \frac{u(Z_{0B}/m_B)}{Z_{0B}/m_B}\right)^2 \right\}. \quad (5.11)
\end{aligned}$$

The uncertainty model for the total energy flow rate of two flow calibrated Coriolis flow meters in parallel can be written as

$$\begin{aligned}
\left(\frac{u(q_e)}{q_e}\right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{m,cal,devA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,devB})}{q_{mB}}\right)^2 + \left(\frac{u(q_{m,cal,refA})}{q_{mA}} + \frac{u(q_{m,cal,refB})}{q_{mB}}\right)^2 \right. \\
& + \left(\frac{u(q_{m,cal,repA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,repB})}{q_{mB}}\right)^2 + \left(\frac{u(q_{m,field,repA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,field,repB})}{q_{mB}}\right)^2 \\
& \left. + \left(\frac{u(q_{m,field,condA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,field,condB})}{q_{mB}}\right)^2 + \left(\frac{u(H_{s,mA})}{H_{s,mA}} + \frac{u(H_{s,mB})}{H_{s,mB}}\right)^2 \right\}. \quad (5.12)
\end{aligned}$$

If the two flow meters are not calibrated at the same time and location:

The uncertainty model for the total mass flow rate of two flow calibrated Coriolis flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned} \left(\frac{u(q_m)}{q_m} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{m,cal,devA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,devB})}{q_{mB}} \right)^2 + \left(\frac{u(q_{m,cal,refA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,refB})}{q_{mB}} \right)^2 \right. \\ & + \left(\frac{u(q_{m,cal,reptA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,reptB})}{q_{mB}} \right)^2 + \left(\frac{u(q_{m,field,reptA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,field,reptB})}{q_{mB}} \right)^2 \\ & \left. + \left(\frac{u(q_{m,field,condA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,field,condB})}{q_{mB}} \right)^2 \right\}. \end{aligned} \quad (5.13)$$

The uncertainty model for the total standard volume flow rate of two flow calibrated Coriolis flow meters in parallel can be written as

$$\begin{aligned} \left(\frac{u(q_{v0})}{q_{v0}} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{m,cal,devA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,devB})}{q_{mB}} \right)^2 + \left(\frac{u(q_{m,cal,refA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,refB})}{q_{mB}} \right)^2 \right. \\ & + \left(\frac{u(q_{m,cal,reptA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,reptB})}{q_{mB}} \right)^2 + \left(\frac{u(q_{m,field,reptA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,field,reptB})}{q_{mB}} \right)^2 \\ & \left. + \left(\frac{u(q_{m,field,condA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,field,condB})}{q_{mB}} \right)^2 + \left(\frac{u(Z_{0A}/m_A)}{Z_{0A}/m_A} + \frac{u(Z_{0B}/m_B)}{Z_{0B}/m_B} \right)^2 \right\}. \end{aligned} \quad (5.14)$$

The uncertainty model for the total energy flow rate of two flow calibrated Coriolis flow meters in parallel can be written as

$$\begin{aligned} \left(\frac{u(q_e)}{q_e} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{m,cal,devA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,devB})}{q_{mB}} \right)^2 + \left(\frac{u(q_{m,cal,refA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,refB})}{q_{mB}} \right)^2 \right. \\ & + \left(\frac{u(q_{m,cal,reptA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,reptB})}{q_{mB}} \right)^2 + \left(\frac{u(q_{m,field,reptA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,field,reptB})}{q_{mB}} \right)^2 \\ & \left. + \left(\frac{u(q_{m,field,condA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,field,condB})}{q_{mB}} \right)^2 + \left(\frac{u(H_{s,mA})}{H_{s,mA}} + \frac{u(H_{s,mB})}{H_{s,mB}} \right)^2 \right\}. \end{aligned} \quad (5.15)$$

5.6 Two flow meters in series

When two Coriolis flow meters are installed in series, the operator can either use one as master and the other just as a check for quality assurance purposes. In that case the uncertainty analysis for one flow meter alone will be the valid one.

This section covers the case when the average flow rate from the two meters is to be used.

5.6.1 Correlation classification

The generic uncertainty model for two flow meters in series is given in Section B 3.

Based on the results of the uncertainty model development in Appendix B, it is necessary to classify all uncertainty contributions as either correlated or uncorrelated between the two flow meters. The following assumptions and evaluations have been made in order to classify the correlations:

- **Calibration uncertainty**
 - *Uncertainty of the correction factor estimate (the adjustment after deviations between flow meter and reference measurement at the flow laboratory are established):* It is assumed that this uncertainty contribution is **uncorrelated** as each meter will have its own deviation curve, and possible errors due to linear interpolation in such a deviation curve are not likely to repeat between different meters.
 - *Uncertainty of the reference measurement at the flow laboratory:* If the two flow meters are calibrated at the same time at the same location, it is likely that this uncertainty contribution is **correlated**, as the flow meters are compared to the same reference. In other cases it is likely that it is **uncorrelated**. In the uncertainty program it is possible to specify whether the flow meters are calibrated at the same time and location or not.
 - *Repeatability, including both the Coriolis flow meter to be calibrated and the reference measurement:* This represents random variations, and will thus be **uncorrelated** between the two flow meters.
- **Field uncertainty**
 - *Repeatability of the flow meter under field operation:* this represents random variations, and will thus be **uncorrelated** between the two flow meters.
 - *Uncertainty due to changes of conditions from flow calibration to field operation:* It is here assumed that this is **uncorrelated**. This is because the upstream of the two meters will affect the flow conditions of the downstream meter. Therefore it is likely that they may be affected differently by changed conditions from calibration to field.
- **Gas parameters**
 - *The uncertainty of the fraction of standard compressibility to molar mass* is used in the uncertainty model for standard volume flow rate. As it is assumed that the same gas composition is used for both flow meters, this parameter is **correlated**.
 - *The uncertainty of the mass based superior calorific value* is used in the uncertainty model for energy flow rate. As it is assumed that the same gas composition is used for both flow meters, this parameter is **correlated**.

5.6.2 Specific uncertainty models

Based on the uncertainty models for one flow calibrated Coriolis meter (mass flow rate Eq. (5.7), standard volume flow rate Eq. (5.8) and energy flow rate Eq. (5.9)), the general model for combining these uncertainty models into a model for two in series (Section B 3) and the classification of uncertainty contributions as either correlated or uncorrelated, the uncertainty models for two flow meters in parallel can be found.

If the two flow meters are calibrated at the same time and location:

The uncertainty model for the average mass flow rate of two flow calibrated Coriolis flow meters in series (meter A and meter B) can be written as

$$\begin{aligned} \left(\frac{u(q_m)}{q_m} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{m,cal,devA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,devB})}{q_{mB}} \right)^2 + \left(\frac{u(q_{m,cal,refA})}{q_{mA}} + \frac{u(q_{m,cal,refB})}{q_{mB}} \right)^2 \right. \\ & + \left(\frac{u(q_{m,cal,repA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,repB})}{q_{mb}} \right)^2 + \left(\frac{u(q_{m,field,repA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,field,repB})}{q_{mB}} \right)^2 \\ & \left. + \left(\frac{u(q_{m,field,condA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,field,condA})}{q_{mA}} \right)^2 \right\}. \end{aligned} \quad (5.16)$$

The uncertainty model for the average standard volume flow rate of two flow calibrated Coriolis flow meters in series can be written as

$$\begin{aligned} \left(\frac{u(q_{v0})}{q_{v0}} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{m,cal,devA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,devB})}{q_{mB}} \right)^2 + \left(\frac{u(q_{m,cal,refA})}{q_{mA}} + \frac{u(q_{m,cal,refB})}{q_{mB}} \right)^2 \right. \\ & + \left(\frac{u(q_{m,cal,repA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,repB})}{q_{mb}} \right)^2 + \left(\frac{u(q_{m,field,repA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,field,repB})}{q_{mB}} \right)^2 \\ & \left. + \left(\frac{u(q_{m,field,condA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,field,condA})}{q_{mA}} \right)^2 + \left(\frac{u(Z_{0A}/m_A)}{Z_{0A}/m_A} + \frac{u(Z_{0B}/m_B)}{Z_{0B}/m_B} \right)^2 \right\}. \end{aligned} \quad (5.17)$$

The uncertainty model for the average energy flow rate of two flow calibrated Coriolis flow meters in series can be written as

$$\begin{aligned} \left(\frac{u(q_e)}{q_e} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{m,cal,devA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,devB})}{q_{mB}} \right)^2 + \left(\frac{u(q_{m,cal,refA})}{q_{mA}} + \frac{u(q_{m,cal,refB})}{q_{mB}} \right)^2 \right. \\ & + \left(\frac{u(q_{m,cal,repA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,cal,repB})}{q_{mb}} \right)^2 + \left(\frac{u(q_{m,field,repA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,field,repB})}{q_{mB}} \right)^2 \\ & \left. + \left(\frac{u(q_{m,field,condA})}{q_{mA}} \right)^2 + \left(\frac{u(q_{m,field,condA})}{q_{mA}} \right)^2 + \left(\frac{u(H_{s,mA})}{H_{s,mA}} + \frac{u(H_{s,mB})}{H_{s,mB}} \right)^2 \right\}. \end{aligned} \quad (5.18)$$

If the two flow meters are not calibrated at the same time and location:

The uncertainty model for the average mass flow rate of two flow calibrated Coriolis flow meters in series (meter A and meter B) can be written as

$$\begin{aligned}
\left(\frac{u(q_m)}{q_m}\right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{m,cal,devA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,devB})}{q_{mB}}\right)^2 + \left(\frac{u(q_{m,cal,refA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,refB})}{q_{mB}}\right)^2 \right. \\
& + \left(\frac{u(q_{m,cal,repA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,repB})}{q_{mB}}\right)^2 + \left(\frac{u(q_{m,field,repA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,field,repB})}{q_{mB}}\right)^2 \\
& \left. + \left(\frac{u(q_{m,field,condA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,field,condB})}{q_{mB}}\right)^2 \right\}. \quad (5.19)
\end{aligned}$$

The uncertainty model for the average standard volume flow rate of two flow calibrated Coriolis flow meters in series can be written as

$$\begin{aligned}
\left(\frac{u(q_{v0})}{q_{v0}}\right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{m,cal,devA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,devB})}{q_{mB}}\right)^2 + \left(\frac{u(q_{m,cal,refA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,refB})}{q_{mB}}\right)^2 \right. \\
& + \left(\frac{u(q_{m,cal,repA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,repB})}{q_{mB}}\right)^2 + \left(\frac{u(q_{m,field,repA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,field,repB})}{q_{mB}}\right)^2 \\
& \left. + \left(\frac{u(q_{m,field,condA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,field,condB})}{q_{mB}}\right)^2 + \left(\frac{u(Z_{0A}/m_A)}{Z_{0A}/m_A} + \frac{u(Z_{0B}/m_B)}{Z_{0B}/m_B}\right)^2 \right\}. \quad (5.20)
\end{aligned}$$

The uncertainty model for the average energy flow rate of two flow calibrated Coriolis flow meters in series can be written as

$$\begin{aligned}
\left(\frac{u(q_e)}{q_e}\right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{m,cal,devA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,devB})}{q_{mB}}\right)^2 + \left(\frac{u(q_{m,cal,refA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,refB})}{q_{mB}}\right)^2 \right. \\
& + \left(\frac{u(q_{m,cal,repA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,cal,repB})}{q_{mB}}\right)^2 + \left(\frac{u(q_{m,field,repA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,field,repB})}{q_{mB}}\right)^2 \\
& \left. + \left(\frac{u(q_{m,field,condA})}{q_{mA}}\right)^2 + \left(\frac{u(q_{m,field,condB})}{q_{mB}}\right)^2 + \left(\frac{u(H_{s,mA})}{H_{s,mA}} + \frac{u(H_{s,mB})}{H_{s,mB}}\right)^2 \right\}. \quad (5.21)
\end{aligned}$$

6 USM fiscal metering stations

In this chapter, uncertainty models for mass flow rate, standard volume flow rate and energy flow rate for an ultrasonic multipath flow metering station are presented. The work is a generalization of the work in [Lunde et al, 2002], where now more set-ups of the metering station are covered.

In Section 6.1 the set-up of the metering station is given. In Section 6.2 the functional relationship for the actual volume flow rate, mass flow rate, standard volume flow rate and energy flow rate for a metering station with one ultrasonic flow meter is presented. Section 6.3 gives the uncertainty model for the actual volume flow rate for a single ultrasonic flow meter. In Section 6.4 this is extended to uncertainty models also for mass flow rate, standard volume flow rate and energy flow rate. Section 6.5 gives the uncertainty model for the total flow rates from two ultrasonic flow meters in parallel, and Section 6.6 for the average flow rates from two ultrasonic flow meters in series.

6.1 Description of metering station

The ultrasonic metering station consists of an ultrasonic multipath flow meter (giving primarily the actual volume flow rate). In addition, pressure and temperature is measured. Density is either measured by a densitometer or calculated based on a gas composition. Furthermore, compressibility and calorific value are calculated based on a gas composition. There are three options covered for the gas composition:

- A given, fixed composition.
- Gas composition measured by online gas chromatograph.
- Gas composition measured by laboratory analysis of spot gas samples.

In addition the cases of two flow meters in parallel and two flow meters in series are covered. In that case each meter has its own pressure and temperature measurements, and when densitometers are in use, each meter has its own dedicated densitometer. It is assumed that the same gas composition is used for both flow meters.

6.2 Functional relationship

6.2.1 Actual volume flow rate, flow calibrated USM meter

The ultrasonic multipath flow meter measures the actual volume flow rate as its primary output. Typically, the ultrasonic flow meter will be flow calibrated. Thus, an adjustment of the flow meter may be carried out.

The flow calibration is carried by comparing the actual volume flow rate as output from the ultrasonic flow meter with the similar reading from a reference measurement. This is carried out at a set of N different flow rates.

The details are covered in Appendix A, where “ x ” is replaced by “ v ” and “*Meter*” is replaced by “*USM*” in the index of the flow rate q in the formulas. Three different ways of correcting the flow meter are covered:

- (i) no correction,
- (ii) a constant percentage correction,
- (iii) linear interpolation.

Appendix A describes the percentage deviation that is corrected (" p ") in all these three cases, and how this is converted to a correction factor K .

It should, however, be commented that the third case (linear interpolation) provides a correction such that the flow meter's flow rate will be corrected to the reference meter flow rate, when the flow rate is equal to any of the flow rates used in the flow calibration. This case is therefore in agreement with the Norwegian Petroleum Directorate Measurement Regulations [NPD], where one requirement in Section 8 is that "*The measurement system shall be designed so that systematic measurement errors are avoided or compensated for*". Using case (i) and (ii) is not in agreement with this requirement.

6.2.2 Mass, standard volume and energy flow rate, flow calibrated USM meter

In the previous subsection it is described how the actual volume flow rate from a flow calibrated ultrasonic flow meter is found. It will here be shown how the mass, standard volume and energy flow rates are found. These calculations are different depending on the set-up of the metering station. First the case where a densitometer is in use will be presented. Thereafter the case where a densitometer is not in use will be presented.

Densitometer in use:

The mass flow rate is found by multiplication of the actual volume flow rate with the measured density (at line conditions):

$$q_m = \rho q_v. \quad (6.1)$$

In order to find the standard volume flow rate, a pressure and temperature correction of the actual volume flow rate must be carried out. In addition, the change in compressibility between line and standard condition must be adjusted for. This gives the following expression:

$$q_{v0} = \frac{P Z_0 T_0}{P_0 Z T} q_v. \quad (6.2)$$

In order to find the compressibility factors, a gas composition is needed, either measured or calculated.

The energy flow rate is obtained by multiplying the mass flow rate by the mass based superior calorific value. This gives the following expression:

$$q_e = H_{s,m} \rho q_v. \quad (6.3)$$

It should be commented here that it is also possible to obtain the energy flow rate by multiplying the standard volume flow rate with the volume based superior calorific value. This will not give the same answer because in that case the measured density from the densitometer will not be used. The uncertainty will also be different. However, that way of establishing the energy flow rate can be analyzed using the option that densitometer is not in use, as the output energy flow rate will be identical to the one described for the case of densitometer not in use.

Densitometer not in use:

In this case, all gas parameters are calculated from the gas composition that must be known either from online gas chromatography, laboratory analysis of gas samples or in other ways.

The density at line conditions is now found from the gas composition, pressure and temperature using the following equation:

$$\rho = \frac{mP}{ZRT} . \quad (6.4)$$

The compressibility factor, Z , is found by using the AGA 8 equation of state.

The mass flow rate is found by multiplication of the actual volume flow rate with the measured density (at line conditions), giving the following expression:

$$q_m = \frac{mP}{ZRT} q_v . \quad (6.5)$$

In order to find the standard volume flow rate, a pressure and temperature correction of the actual volume flow rate must be carried out. In addition, the change in compressibility between line and standard condition must be adjusted for. This gives the following expression:

$$q_{v0} = \frac{PZ_0T_0}{P_0ZT} q_v . \quad (6.6)$$

In order to find the compressibility factors, a gas composition is needed, either measured or calculated.

The energy flow rate is obtained by multiplying the mass flow rate by the mass based superior calorific value. This gives the following expression:

$$q_e = H_{s,m} \frac{mP}{ZRT} q_v . \quad (6.7)$$

6.3 Uncertainty model, actual volume flow rate

The uncertainty of the actual volume flow rate of a flow calibrated ultrasonic meter consists of two general uncertainty contributions

- Calibration uncertainty
- Field uncertainty

Formally, this can be written as follows

$$\left(\frac{u(q_v)}{q_v} \right)^2 = \left(\frac{u(q_{v,cal})}{q_v} \right)^2 + \left(\frac{u(q_{v,field})}{q_v} \right)^2 . \quad (6.8)$$

These two contributions will now be discussed more in detail.

6.3.1 Calibration uncertainty

The calibration uncertainty consists of the following three contributions:

- Uncertainty of the correction factor estimate (the adjustment after deviations between flow meter and reference measurement at the flow laboratory are established).

- Uncertainty of the reference measurement at the flow laboratory.
- Repeatability, including both the ultrasonic flow meter to be calibrated and the reference measurement.

This can be written as

$$\left(\frac{u(q_{v,cal})}{q_v} \right)^2 = \left(\frac{u(q_{v,cal,dev})}{q_v} \right)^2 + \left(\frac{u(q_{v,cal,ref})}{q_v} \right)^2 + \left(\frac{u(q_{v,cal, rept})}{q_v} \right)^2. \quad (6.9)$$

These three terms will now be discussed more in detail.

Uncertainty of the correction factor estimate: This uncertainty contribution is described in Appendix A, where, where “x” is replaced by “v” and “Meter” is replaced by “USM” in the index of the flow rate q in the formulas. It is calculated from the deviation between the ultrasonic flow meter’s actual volume flow rate and the actual volume flow rate measured by the reference meter, at a series of actual volume flow rates. Three adjustment methods for the ultrasonic flow meter are discussed:

- (i) no correction,
- (ii) a constant percentage correction,
- (iii) linear interpolation.

For each of these methods, the actual expression is given in Appendix A for any uncorrected percentage deviation, δp , of the flow meter after adjustment of the ultrasonic flow meter.

As described in Appendix A, the relative standard uncertainty of the correction factor estimate can now be written as

$$\left(\frac{u(q_{m,cal,dev})}{q_m} \right) = \left(\frac{u(K)}{K} \right) = \frac{1}{K} \frac{\partial p}{\partial K} u(p) = \frac{\delta p / \sqrt{3}}{100 + p}. \quad (6.10)$$

Uncertainty of the reference measurement: This term depends on the metering equipment at the flow laboratory. This number is usually found in the calibration certificate. It can depend on the flow rate. Therefore, for actual volume flow rates between the ones used in the flow calibration, a linear interpolation based on the values of this uncertainty at the actual volume flow rates used in flow calibration is used. The relative uncertainty at the highest calibrated flow rate will be used for flow rates above this highest calibrated flow rate. The relative uncertainty at the lowest calibrated flow rate will be used for flow rates below this lowest calibrated flow rate.

Repeatability: This term covers both the repeatability of the ultrasonic flow meter to be calibrated and the reference measurement. It can vary with actual volume flow rate. Therefore, for actual volume flow rates between the ones used in the flow calibration, a linear interpolation based on the values of this repeatability at the actual volume flow rates used in flow calibration is used. The repeatability at the highest calibrated flow rate will be used for flow rates above this highest calibrated flow rate. The repeatability at the lowest calibrated flow rate will be used for flow rates below this lowest calibrated flow rate.

6.3.2 Field uncertainty

The field uncertainty will consist of the following two contributions

- Repeatability of the flow meter under field operation
- Uncertainty due to changes of conditions from flow calibration to field operation

This can be written as

$$\left(\frac{u(q_{v,field})}{q_v} \right)^2 = \left(\frac{u(q_{v,field, rept})}{q_v} \right)^2 + \left(\frac{u(q_{v,field, cond})}{q_v} \right)^2. \quad (6.11)$$

These two terms will now be discussed more in detail.

Repeatability of the flow meter under field operation: This can usually be found in the data sheet of the flow meter, if not own experience is used for establishing the repeatability. It is possible to specify different values on the repeatability for different flow rates. In that case linear interpolation is used for obtaining the repeatability at actual volume flow rates in-between the ones where the repeatability is specified. The repeatability at the highest calibrated flow rate will be used for flow rates above this highest calibrated flow rate. The repeatability at the lowest calibrated flow rate will be used for flow rates below this lowest calibrated flow rate.

Uncertainty due to changes of conditions from flow calibration to field operation: The value of this quantity will depend on the actual installation and on the data sheet of the flow meter. In the program this uncertainty contribution can either be specified directly (overall level) or can be calculated based on more detailed uncertainty input. The latter case is based on the results of [Lunde et al, 2002]. The connection to that work is described in Appendix C.

When overall level is specified, it is possible to specify different values on the relative uncertainty at different flow rates. In that case linear interpolation is used for obtaining the relative uncertainty at actual volume flow rates in-between the ones where it is specified. The relative uncertainty at the highest calibrated flow rate will be used for flow rates above this highest calibrated flow rate. The relative uncertainty at the lowest calibrated flow rate will be used for flow rates below this lowest calibrated flow rate.

When detailed level is specified, this uncertainty term is calculated from the specified input.

6.3.3 Total uncertainty in actual volume flow rate, one flow meter

Based on the two previous sub-sections, the total uncertainty model for the actual volume flow rate from a flow calibrated ultrasonic flow meter can be written as

$$\begin{aligned} \left(\frac{u(q_v)}{q_v} \right)^2 = & \left(\frac{u(q_{v,cal,dev})}{q_v} \right)^2 + \left(\frac{u(q_{v,cal,ref})}{q_v} \right)^2 + \left(\frac{u(q_{v,cal, rept})}{q_v} \right)^2 \\ & + \left(\frac{u(q_{v,field, rept})}{q_v} \right)^2 + \left(\frac{u(q_{v,field, cond})}{q_v} \right)^2. \end{aligned} \quad (6.12)$$

6.4 Uncertainty model, mass, standard volume and energy flow rate

The uncertainty models for the mass, standard volume and energy flow rate depend on whether a densitometer is in use or not. Both cases will be covered.

6.4.1 Densitometer in use

Eq. (6.1) describes the functional relationship between the actual volume flow rate and the mass flow rate. The uncertainty model for the mass flow rate is found to be as

$$\left(\frac{u(q_m)}{q_m}\right)^2 = \left(\frac{u(q_v)}{q_v}\right)^2 + \left(\frac{u(\rho)}{\rho}\right)^2. \quad (6.13)$$

Eq. (6.2) describes the functional relationship between the actual volume flow rate and the standard volume flow rate. The compressibility factors at line and standard conditions depend both on the gas composition, and in order to avoid correlations, the uncertainty model for the standard volume flow rate is written as

$$\left(\frac{u(q_{v0})}{q_{v0}}\right)^2 = \left(\frac{u(q_v)}{q_v}\right)^2 + \left(\frac{u(P)}{P}\right)^2 + \left(\frac{u(T)}{T}\right)^2 + \left(\frac{u(Z/Z_0)}{Z/Z_0}\right)^2. \quad (6.14)$$

Eq. (6.3) describes the functional relationship between the actual volume flow rate and the energy flow rate. The mass based superior calorific value depends on the gas composition, and has thus uncertainty. The uncertainty model for the energy flow rate is written as

$$\left(\frac{u(q_e)}{q_e}\right)^2 = \left(\frac{u(q_v)}{q_v}\right)^2 + \left(\frac{u(\rho)}{\rho}\right)^2 + \left(\frac{u(H_{s,m})}{H_{s,m}}\right)^2. \quad (6.15)$$

6.4.2 Densitometer not in use

Eq. (6.5) describes the functional relationship between the actual volume flow rate and the mass flow rate. The molar mass and the compressibility factor at line conditions depend both on the gas composition, and in order to avoid correlations, the uncertainty model for the mass flow rate is written as

$$\left(\frac{u(q_m)}{q_m}\right)^2 = \left(\frac{u(q_v)}{q_v}\right)^2 + \left(\frac{u(P)}{P}\right)^2 + \left(\frac{u(T)}{T}\right)^2 + \left(\frac{u(m/Z)}{m/Z}\right)^2. \quad (6.16)$$

Eq. (6.6) describes the functional relationship between the actual volume flow rate and the standard volume flow rate. This is identical to Eq. (6.2), valid when a densitometer is in use. Therefore, the uncertainty model for the standard volume flow rate is identical to Eq. (6.14), and is repeated here for completeness:

$$\left(\frac{u(q_{v0})}{q_{v0}}\right)^2 = \left(\frac{u(q_v)}{q_v}\right)^2 + \left(\frac{u(P)}{P}\right)^2 + \left(\frac{u(T)}{T}\right)^2 + \left(\frac{u(Z/Z_0)}{Z/Z_0}\right)^2. \quad (6.17)$$

Eq. (6.7) describes the functional relationship between the actual volume flow rate and the energy flow rate. The superior calorific value, the molar mass and the compressibility factor at line conditions depend all on the gas composition. In order to avoid correlations, the uncertainty model for the energy flow rate is written as

$$\left(\frac{u(q_e)}{q_e}\right)^2 = \left(\frac{u(q_v)}{q_v}\right)^2 + \left(\frac{u(P)}{P}\right)^2 + \left(\frac{u(T)}{T}\right)^2 + \left(\frac{u(H_{s,m} m/Z)}{H_{s,m} m/Z}\right)^2. \quad (6.18)$$

6.5 Two flow meters in parallel

6.5.1 Correlation classification

The generic uncertainty model for two flow meters in parallel is given in Appendix B. The uncertainty model is developed under the assumption that the flow rate is about the same in both pipes.

Based on the results of the uncertainty model development in Section B 2, it is necessary to classify all uncertainty contributions as either correlated or uncorrelated between the two flow meters. The following assumptions and evaluations have been made in order to classify the correlations:

- **Calibration uncertainty**
 - *Uncertainty of the correction factor estimate (the adjustment after deviations between flow meter and reference measurement at the flow laboratory are established):* It is assumed that this uncertainty contribution is **uncorrelated** as each meter will have its own deviation curve, and possible errors due to linear interpolation in such a deviation curve are not likely to repeat between different meters.
 - *Uncertainty of the reference measurement at the flow laboratory:* If the two flow meters are calibrated at the same time at the same location, it is likely that this uncertainty contribution is **correlated**, as the flow meters are compared to the same reference. In other cases it is likely that it is **uncorrelated**. In the uncertainty program it is possible to specify whether the flow meters are calibrated at the same time and location or not.
 - *Repeatability, including both the ultrasonic flow meter to be calibrated and the reference measurement:* This represents random variations, and will thus be **uncorrelated** between the two flow meters.
- **Field uncertainty**
 - *Repeatability of the flow meter under field operation:* this represents random variations, and will thus be **uncorrelated** between the two flow meters.
 - *Uncertainty due to changes of conditions from flow calibration to field operation:* It is here assumed that this is **uncorrelated**. This is because the flow conditions will never be identical in two different pipes, and therefore it is likely that they may be affected differently by changed conditions from calibration to field.
- **Gas parameters**
 - Measured pressure: Each flow meter has its own pressure meter. It is therefore assumed that this effect is **uncorrelated**.
 - Measured temperature: Each flow meter has its own temperature meter. It is therefore assumed that this effect is **uncorrelated**.
 - Measured density: Each flow meter has its own densitometer. It is therefore assumed that this effect is **uncorrelated**.
 - *The uncertainty of the various fractions and products of molar mass, compressibilities and/or calorific value:* As it is assumed that the same gas composition is used for both flow meters, this parameter is **correlated**.

6.5.2 Specific uncertainty model, densitometer in use

Based on the uncertainty models for one flow calibrated ultrasonic flow meter (actual volume flow rate Eq. (6.12), mass flow rate Eq. (6.13), standard volume flow rate Eq. (6.14) and energy flow rate Eq. (6.15)), the general model for combining these uncertainty models into a model for two in parallel (Appendix B) and the classification of uncertainty contributions as either correlated or uncorrelated, the uncertainty models for two flow meters in parallel can be found.

If the two flow meters are calibrated at the same time and location:

The uncertainty model for the total mass flow rate of two flow calibrated ultrasonic flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned} \left(\frac{u(q_m)}{q_m} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} + \frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}} \right)^2 \\ & \left. + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(\rho_A)}{\rho_A} \right)^2 + \left(\frac{u(\rho_B)}{\rho_B} \right)^2 \right\}. \end{aligned} \quad (6.19)$$

The uncertainty model for the total standard volume flow rate of two flow calibrated ultrasonic flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned} \left(\frac{u(q_{v0})}{q_{v0}} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} + \frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}} \right)^2 \\ & + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(P_A)}{P_A} \right)^2 + \left(\frac{u(P_B)}{P_B} \right)^2 \\ & \left. + \left(\frac{u(T_A)}{T_A} \right)^2 + \left(\frac{u(T_B)}{T_B} \right)^2 + \left(\frac{u(Z_A/Z_{0A})}{Z_A/Z_{0A}} + \frac{u(Z_B/Z_{0B})}{Z_B/Z_{0B}} \right)^2 \right\}. \end{aligned} \quad (6.20)$$

The uncertainty model for the total energy flow rate of two flow calibrated ultrasonic flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned} \left(\frac{u(q_e)}{q_e} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} + \frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}} \right)^2 \\ & + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(\rho_A)}{\rho_A} \right)^2 + \left(\frac{u(\rho_B)}{\rho_B} \right)^2 \\ & \left. + \left(\frac{u(H_{s,mA})}{H_{s,mA}} + \frac{u(H_{s,mB})}{H_{s,mB}} \right)^2 \right\}. \end{aligned} \quad (6.21)$$

If the two flow meters are not calibrated at the same time and location:

The uncertainty model for the total mass flow rate of two flow calibrated ultrasonic flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned} \left(\frac{u(q_m)}{q_m} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}} \right)^2 \\ & \left. + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(\rho_A)}{\rho_A} \right)^2 + \left(\frac{u(\rho_B)}{\rho_B} \right)^2 \right\}. \end{aligned} \quad (6.22)$$

The uncertainty model for the total standard volume flow rate of two flow calibrated ultrasonic flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned} \left(\frac{u(q_{v0})}{q_{v0}} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}} \right)^2 \\ & + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(P_A)}{P_A} \right)^2 + \left(\frac{u(P_B)}{P_B} \right)^2 \\ & \left. + \left(\frac{u(T_A)}{T_A} \right)^2 + \left(\frac{u(T_B)}{T_B} \right)^2 + \left(\frac{u(Z_A/Z_{0A})}{Z_A/Z_{0A}} + \frac{u(Z_B/Z_{0B})}{Z_B/Z_{0B}} \right)^2 \right\}. \end{aligned} \quad (6.23)$$

The uncertainty model for the total energy flow rate of two flow calibrated ultrasonic flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned}
\left(\frac{u(q_e)}{q_e}\right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}}\right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,refB})}{q_{vB}}\right)^2 \right. \\
& + \left(\frac{u(q_{v,cal,repA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}}\right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}}\right)^2 \\
& + \left(\frac{u(q_{v,field,conA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}}\right)^2 + \left(\frac{u(\rho_A)}{\rho_A}\right)^2 + \left(\frac{u(\rho_B)}{\rho_B}\right)^2 \\
& \left. + \left(\frac{u(H_{s,mA})}{H_{s,mA}} + \frac{u(H_{s,mB})}{H_{s,mB}}\right)^2 \right\}.
\end{aligned} \tag{6.24}$$

6.5.3 Specific uncertainty model, densitometer not in use

Based on the uncertainty models for one flow calibrated ultrasonic flow meter (actual volume flow rate Eq. (6.12), mass flow rate Eq. (6.16), standard volume flow rate Eq. (6.17) and energy flow rate Eq. (6.18)), the general model for combining these uncertainty models into a model for two in parallel (Appendix B) and the classification of uncertainty contributions as either correlated or uncorrelated, the uncertainty models for two flow meters in parallel can be found.

If the two flow meters are calibrated at the same time and location:

The uncertainty model for the total mass flow rate of two flow calibrated ultrasonic flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned}
\left(\frac{u(q_m)}{q_m}\right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}}\right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} + \frac{u(q_{v,cal,refB})}{q_{vB}}\right)^2 \right. \\
& + \left(\frac{u(q_{v,cal,repA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}}\right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}}\right)^2 \\
& + \left(\frac{u(q_{v,field,conA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}}\right)^2 + \left(\frac{u(P_A)}{P_A}\right)^2 + \left(\frac{u(P_B)}{P_B}\right)^2 \\
& \left. + \left(\frac{u(T_A)}{T_A}\right)^2 + \left(\frac{u(T_B)}{T_B}\right)^2 + \left(\frac{u(m_A/Z_A)}{m_A/Z_A} + \frac{u(m_B/Z_B)}{m_B/Z_B}\right)^2 \right\}.
\end{aligned} \tag{6.25}$$

As for the case of a single ultrasonic flow meter, the uncertainty model for the total standard volume flow rate of two flow calibrated ultrasonic flow meters in parallel (meter A and meter B) is equal to the similar uncertainty model when densitometer is in use. It is repeated here for completeness:

$$\begin{aligned} \left(\frac{u(q_{v0})}{q_{v0}} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} + \frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}} \right)^2 \\ & + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(P_A)}{P_A} \right)^2 + \left(\frac{u(P_B)}{P_B} \right)^2 \\ & \left. + \left(\frac{u(T_A)}{T_A} \right)^2 + \left(\frac{u(T_B)}{T_B} \right)^2 + \left(\frac{u(Z_A/Z_{0A})}{Z_A/Z_{0A}} + \frac{u(Z_B/Z_{0B})}{Z_B/Z_{0B}} \right)^2 \right\}. \end{aligned} \quad (6.26)$$

The uncertainty model for the total energy flow rate of two flow calibrated ultrasonic flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned} \left(\frac{u(q_e)}{q_e} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} + \frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}} \right)^2 \\ & + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(P_A)}{P_A} \right)^2 + \left(\frac{u(P_B)}{P_B} \right)^2 \\ & \left. + \left(\frac{u(T_A)}{T_A} \right)^2 + \left(\frac{u(T_B)}{T_B} \right)^2 + \left(\frac{u(H_{s,mA}m_A/Z_A)}{H_{s,mA}m_A/Z_A} + \frac{u(H_{s,mB}m_B/Z_B)}{H_{s,mB}m_B/Z_B} \right)^2 \right\}. \end{aligned} \quad (6.27)$$

If the two flow meters are not calibrated at the same time and location:

The uncertainty model for the total mass flow rate of two flow calibrated ultrasonic flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned} \left(\frac{u(q_m)}{q_m} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}} \right)^2 \\ & + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(P_A)}{P_A} \right)^2 + \left(\frac{u(P_B)}{P_B} \right)^2 \\ & \left. + \left(\frac{u(T_A)}{T_A} \right)^2 + \left(\frac{u(T_B)}{T_B} \right)^2 + \left(\frac{u(m_A/Z_A)}{m_A/Z_A} + \frac{u(m_B/Z_B)}{m_B/Z_B} \right)^2 \right\}. \end{aligned} \quad (6.28)$$

As for the case of a single ultrasonic flow meter, the uncertainty model for the total standard volume flow rate of two flow calibrated ultrasonic flow meters in parallel (meter A and meter B) is equal to the similar uncertainty model when densitometer is in use. It is repeated here for completeness:

$$\begin{aligned} \left(\frac{u(q_{v0})}{q_{v0}} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,reprA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,reprB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,reprA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,reprB})}{q_{vB}} \right)^2 \\ & + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(P_A)}{P_A} \right)^2 + \left(\frac{u(P_B)}{P_B} \right)^2 \\ & \left. + \left(\frac{u(T_A)}{T_A} \right)^2 + \left(\frac{u(T_B)}{T_B} \right)^2 + \left(\frac{u(Z_A/Z_{0A})}{Z_A/Z_{0A}} + \frac{u(Z_B/Z_{0B})}{Z_B/Z_{0B}} \right)^2 \right\}. \end{aligned} \quad (6.29)$$

The uncertainty model for the total energy flow rate of two flow calibrated ultrasonic flow meters in parallel (meter A and meter B) can be written as

$$\begin{aligned} \left(\frac{u(q_e)}{q_e} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,reprA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,reprB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,reprA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,reprB})}{q_{vB}} \right)^2 \\ & + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(P_A)}{P_A} \right)^2 + \left(\frac{u(P_B)}{P_B} \right)^2 \\ & \left. + \left(\frac{u(T_A)}{T_A} \right)^2 + \left(\frac{u(T_B)}{T_B} \right)^2 + \left(\frac{u(H_{s,mA}m_A/Z_A)}{H_{s,mA}m_A/Z_A} + \frac{u(H_{s,mB}m_B/Z_B)}{H_{s,mB}m_B/Z_B} \right)^2 \right\}. \end{aligned} \quad (6.30)$$

6.6 Two flow meters in series

When two ultrasonic flow meters are installed in series, the operator can either use one as master and the other just as a check for quality assurance purposes. In that case the uncertainty analysis for one flow meter alone will be the valid one.

This section covers the case when the average flow rate from the two meters is to be used.

6.6.1 Correlation classification

The generic uncertainty model for two flow meters in series is given in Appendix B.

Based on the results of the uncertainty model development in Section B 3, it is necessary to classify all uncertainty contributions as either correlated or uncorrelated between the two flow meters. The following assumptions and evaluations have been made in order to classify the correlations:

- **Calibration uncertainty**

- *Uncertainty of the correction factor estimate (the adjustment after deviations between flow meter and reference measurement at the flow laboratory are established):* It is assumed that this uncertainty contribution is **uncorrelated** as each meter will have its own deviation curve, and possible errors due to linear interpolation in such a deviation curve are not likely to repeat between different meters.
- *Uncertainty of the reference measurement at the flow laboratory:* If the two flow meters are calibrated at the same time at the same location, it is likely that this uncertainty contribution is **correlated**, as the flow meters are compared to the same reference. In other cases it is likely that it is **uncorrelated**. In the uncertainty program it is possible to specify whether the flow meters are calibrated at the same time and location or not.
- *Repeatability, including both the ultrasonic flow meter to be calibrated and the reference measurement:* This represents random variations, and will thus be **uncorrelated** between the two flow meters.

- **Field uncertainty**

- *Repeatability of the flow meter under field operation:* this represents random variations, and will thus be **uncorrelated** between the two flow meters.
- *Uncertainty due to changes of conditions from flow calibration to field operation:* It is here assumed that this is **uncorrelated**. This is because the flow conditions will never be identical due to different straight upstream length for the two meters, and also because the transducer ports of the upstream flow meter may affect the downstream flow meter. Therefore it is likely that they may be affected differently by changed conditions from calibration to field.

- **Gas parameters**

- Measured pressure: Each flow meter has its own pressure meter. It is therefore assumed that this effect is **uncorrelated**.
- Measured temperature: Each flow meter has its own temperature meter. It is therefore assumed that this effect is **uncorrelated**.
- Measured density: Each flow meter has its own densitometer. It is therefore assumed that this effect is **uncorrelated**.
- *The uncertainty of the various fractions and products of molar mass, compressibilities and/or calorific value:* As it is assumed that the same gas composition is used for both flow meters, this parameter is **correlated**.

6.6.2 Specific uncertainty model, densitometer in use

Based on the uncertainty models for one flow calibrated ultrasonic flow meter (actual volume flow rate Eq. (6.12), mass flow rate Eq. (6.13), standard volume flow rate Eq. (6.14) and energy flow rate Eq. (6.15)), the general model for combining these uncertainty models into a model for the average flow rate measured by two ultrasonic flow meters in series (Section B 3) and the classification of uncertainty contributions as either correlated or uncorrelated, the uncertainty models for two flow meters in series can be found.

If the two flow meters are calibrated at the same time and location:

The uncertainty model for the average mass flow rate of two flow calibrated ultrasonic flow meters in series (meter A and meter B) can be written as

$$\begin{aligned}
\left(\frac{u(q_m)}{q_m}\right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}}\right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} + \frac{u(q_{v,cal,refB})}{q_{vB}}\right)^2 \right. \\
& + \left(\frac{u(q_{v,cal,repA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}}\right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}}\right)^2 \\
& \left. + \left(\frac{u(q_{v,field,conA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}}\right)^2 + \left(\frac{u(\rho_A)}{\rho_A}\right)^2 + \left(\frac{u(\rho_B)}{\rho_B}\right)^2 \right\}.
\end{aligned} \quad (6.31)$$

The uncertainty model for the average standard volume flow rate of two flow calibrated ultrasonic flow meters in series (meter A and meter B) can be written as

$$\begin{aligned}
\left(\frac{u(q_{v0})}{q_{v0}}\right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}}\right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} + \frac{u(q_{v,cal,refB})}{q_{vB}}\right)^2 \right. \\
& + \left(\frac{u(q_{v,cal,repA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}}\right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}}\right)^2 \\
& + \left(\frac{u(q_{v,field,conA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}}\right)^2 + \left(\frac{u(P_A)}{P_A}\right)^2 + \left(\frac{u(P_B)}{P_B}\right)^2 \\
& \left. + \left(\frac{u(T_A)}{T_A}\right)^2 + \left(\frac{u(T_B)}{T_B}\right)^2 + \left(\frac{u(Z_A/Z_{0A})}{Z_A/Z_{0A}} + \frac{u(Z_B/Z_{0B})}{Z_B/Z_{0B}}\right)^2 \right\}.
\end{aligned} \quad (6.32)$$

The uncertainty model for the average energy flow rate of two flow calibrated ultrasonic flow meters in series (meter A and meter B) can be written as

$$\begin{aligned}
\left(\frac{u(q_e)}{q_e}\right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}}\right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} + \frac{u(q_{v,cal,refB})}{q_{vB}}\right)^2 \right. \\
& + \left(\frac{u(q_{v,cal,repA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}}\right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}}\right)^2 \\
& + \left(\frac{u(q_{v,field,conA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}}\right)^2 + \left(\frac{u(\rho_A)}{\rho_A}\right)^2 + \left(\frac{u(\rho_B)}{\rho_B}\right)^2 \\
& \left. + \left(\frac{u(H_{s,mA})}{H_{s,mA}} + \frac{u(H_{s,mB})}{H_{s,mB}}\right)^2 \right\}.
\end{aligned} \quad (6.33)$$

If the two flow meters are not calibrated at the same time and location:

The uncertainty model for the average mass flow rate of two flow calibrated ultrasonic flow meters in series (meter A and meter B) can be written as

$$\begin{aligned} \left(\frac{u(q_m)}{q_m} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}} \right)^2 \\ & \left. + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(\rho_A)}{\rho_A} \right)^2 + \left(\frac{u(\rho_B)}{\rho_B} \right)^2 \right\}. \end{aligned} \quad (6.34)$$

The uncertainty model for the average standard volume flow rate of two flow calibrated ultrasonic flow meters in series (meter A and meter B) can be written as

$$\begin{aligned} \left(\frac{u(q_{v0})}{q_{v0}} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}} \right)^2 \\ & + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(P_A)}{P_A} \right)^2 + \left(\frac{u(P_B)}{P_B} \right)^2 \\ & \left. + \left(\frac{u(T_A)}{T_A} \right)^2 + \left(\frac{u(T_B)}{T_B} \right)^2 + \left(\frac{u(Z_A/Z_{0A})}{Z_A/Z_{0A}} + \frac{u(Z_B/Z_{0B})}{Z_B/Z_{0B}} \right)^2 \right\}. \end{aligned} \quad (6.35)$$

The uncertainty model for the average energy flow rate of two flow calibrated ultrasonic flow meters in series (meter A and meter B) can be written as

$$\begin{aligned} \left(\frac{u(q_e)}{q_e} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}} \right)^2 \\ & + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(\rho_A)}{\rho_A} \right)^2 + \left(\frac{u(\rho_B)}{\rho_B} \right)^2 \\ & \left. + \left(\frac{u(H_{s,mA})}{H_{s,mA}} + \frac{u(H_{s,mB})}{H_{s,mB}} \right)^2 \right\}. \end{aligned} \quad (6.36)$$

6.6.3 Specific uncertainty model, densitometer not in use

Based on the uncertainty models for one flow calibrated ultrasonic flow meter (actual volume flow rate Eq. (6.12), mass flow rate Eq. (6.16), standard volume flow rate Eq. (6.17) and energy flow rate Eq. (6.18)), the general model for combining these uncertainty models into a model for the average flow rate

measured by two ultrasonic flow meters in series (Appendix B) and the classification of uncertainty contributions as either correlated or uncorrelated, the uncertainty models for two flow meters in parallel can be found.

If the two flow meters are calibrated at the same time and location:

The uncertainty model for the average mass flow rate of two flow calibrated ultrasonic flow meters in series (meter A and meter B) can be written as

$$\begin{aligned} \left(\frac{u(q_m)}{q_m} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} + \frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}} \right)^2 \\ & + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(P_A)}{P_A} \right)^2 + \left(\frac{u(P_B)}{P_B} \right)^2 \\ & \left. + \left(\frac{u(T_A)}{T_A} \right)^2 + \left(\frac{u(T_B)}{T_B} \right)^2 + \left(\frac{u(m_A/Z_A)}{m_A/Z_A} + \frac{u(m_B/Z_B)}{m_B/Z_B} \right)^2 \right\}. \end{aligned} \quad (6.37)$$

As for the case of a single ultrasonic flow meter and two ultrasonic flow meters in parallel, the uncertainty model for the average standard volume flow rate of two flow calibrated ultrasonic flow meters in series (meter A and meter B) is equal to the similar uncertainty model when densitometer is in use. It is repeated here for completeness:

$$\begin{aligned} \left(\frac{u(q_{v0})}{q_{v0}} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} + \frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\ & + \left(\frac{u(q_{v,cal,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,repB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,repA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,repB})}{q_{vB}} \right)^2 \\ & + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(P_A)}{P_A} \right)^2 + \left(\frac{u(P_B)}{P_B} \right)^2 \\ & \left. + \left(\frac{u(T_A)}{T_A} \right)^2 + \left(\frac{u(T_B)}{T_B} \right)^2 + \left(\frac{u(Z_A/Z_{0A})}{Z_A/Z_{0A}} + \frac{u(Z_B/Z_{0B})}{Z_B/Z_{0B}} \right)^2 \right\}. \end{aligned} \quad (6.38)$$

The uncertainty model for the average energy flow rate of two flow calibrated ultrasonic flow meters in series (meter A and meter B) can be written as

$$\begin{aligned}
 \left(\frac{u(q_e)}{q_e} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} + \frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\
 & + \left(\frac{u(q_{v,cal,reprA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,reprB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,reprA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,reprB})}{q_{vB}} \right)^2 \\
 & + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(P_A)}{P_A} \right)^2 + \left(\frac{u(P_B)}{P_B} \right)^2 \\
 & \left. + \left(\frac{u(T_A)}{T_A} \right)^2 + \left(\frac{u(T_B)}{T_B} \right)^2 + \left(\frac{u(H_{s,mA}m_A/Z_A)}{H_{s,mA}m_A/Z_A} + \frac{u(H_{s,mB}m_B/Z_B)}{H_{s,mB}m_B/Z_B} \right)^2 \right\}.
 \end{aligned} \tag{6.39}$$

If the two flow meters are not calibrated at the same time and location:

The uncertainty model for the average mass flow rate of two flow calibrated ultrasonic flow meters in series (meter A and meter B) can be written as

$$\begin{aligned}
 \left(\frac{u(q_m)}{q_m} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,refB})}{q_{vB}} \right)^2 \right. \\
 & + \left(\frac{u(q_{v,cal,reprA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,cal,reprB})}{q_{vB}} \right)^2 + \left(\frac{u(q_{v,field,reprA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,reprB})}{q_{vB}} \right)^2 \\
 & + \left(\frac{u(q_{v,field,conA})}{q_{vA}} \right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}} \right)^2 + \left(\frac{u(P_A)}{P_A} \right)^2 + \left(\frac{u(P_B)}{P_B} \right)^2 \\
 & \left. + \left(\frac{u(T_A)}{T_A} \right)^2 + \left(\frac{u(T_B)}{T_B} \right)^2 + \left(\frac{u(m_A/Z_A)}{m_A/Z_A} + \frac{u(m_B/Z_B)}{m_B/Z_B} \right)^2 \right\}.
 \end{aligned} \tag{6.40}$$

As for the case of a single ultrasonic flow meter and two ultrasonic flow meters in parallel, the uncertainty model for the average standard volume flow rate of two flow calibrated ultrasonic flow meters in series (meter A and meter B) is equal to the similar uncertainty model when densitometer is in use. It is repeated here for completeness:

$$\begin{aligned}
\left(\frac{u(q_{v0})}{q_{v0}}\right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}}\right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,refB})}{q_{vB}}\right)^2 \right. \\
& + \left(\frac{u(q_{v,cal,reptA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,reptB})}{q_{vB}}\right)^2 + \left(\frac{u(q_{v,field,reptA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,field,reptB})}{q_{vB}}\right)^2 \\
& + \left(\frac{u(q_{v,field,conA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}}\right)^2 + \left(\frac{u(P_A)}{P_A}\right)^2 + \left(\frac{u(P_B)}{P_B}\right)^2 \\
& \left. + \left(\frac{u(T_A)}{T_A}\right)^2 + \left(\frac{u(T_B)}{T_B}\right)^2 + \left(\frac{u(Z_A/Z_{0A})}{Z_A/Z_{0A}} + \frac{u(Z_B/Z_{0B})}{Z_B/Z_{0B}}\right)^2 \right\}.
\end{aligned} \tag{6.41}$$

The uncertainty model for the average energy flow rate of two flow calibrated ultrasonic flow meters in series (meter A and meter B) can be written as

$$\begin{aligned}
\left(\frac{u(q_e)}{q_e}\right)^2 = \frac{1}{4} & \left\{ \left(\frac{u(q_{v,cal,devA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,devB})}{q_{vB}}\right)^2 + \left(\frac{u(q_{v,cal,refA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,refB})}{q_{vB}}\right)^2 \right. \\
& + \left(\frac{u(q_{v,cal,reptA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,cal,reptB})}{q_{vB}}\right)^2 + \left(\frac{u(q_{v,field,reptA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,field,reptB})}{q_{vB}}\right)^2 \\
& + \left(\frac{u(q_{v,field,conA})}{q_{vA}}\right)^2 + \left(\frac{u(q_{v,field,condB})}{q_{vB}}\right)^2 + \left(\frac{u(P_A)}{P_A}\right)^2 + \left(\frac{u(P_B)}{P_B}\right)^2 \\
& \left. + \left(\frac{u(T_A)}{T_A}\right)^2 + \left(\frac{u(T_B)}{T_B}\right)^2 + \left(\frac{u(H_{s,mA}m_A/Z_A)}{H_{s,mA}m_A/Z_A} + \frac{u(H_{s,mB}m_B/Z_B)}{H_{s,mB}m_B/Z_B}\right)^2 \right\}.
\end{aligned} \tag{6.42}$$

7 GasMetering Silverlight Application

NOTE: since support for the Silverlight runtime will end 12. October 2021, users should transition to the new web application before this date, see Chapter 8.

This chapter documents the GasMetering Silverlight application for carrying out uncertainty analyses based on the uncertainty models described in this report. It should here be emphasised that this report is a documentation of the uncertainty models and the corresponding web-based calculation tool. Therefore, the example input values in that calculation tool are just examples, and should not be regarded as recommended values by NFOGM, NORCE, NPD or any other party.

7.1 Software platform

The «Gasmetering» application is implemented in the “Microsoft Silverlight 5” framework, a subset of “Microsoft .Net” that can be installed in a web browser. This framework facilitates running applications with rich functionality in the web browser, without need for installation and with high security. When the user visits a web page the complete application will be downloaded and run securely without need for any further communication with the web server. The application is stored in the web browser cache and will only be downloaded again if there is a new version available.

The choice of Silverlight was based on the available implementation language (C#) and reuse of existing source code base. It could be feasible to implement the application on other platforms in the future.

Microsoft Silverlight 5 is in 2020 only available for Windows using Internet Explorer 11 and will be supported and updated until 12. October 2021. After this date Silverlight applications will continue to work but will not receive quality or security updates. However, due to typical corporate security policies, this implies that for most users the GasMetering Silverlight application will effectively be unavailable at this date.

7.2 Installation and use

The web address for the application will be published on nfogm.no. By visiting the published address, the complete application will be downloaded and run. The download is about 1 MB and will only be downloaded again if there is a newer version available. If the client PC does not have “Microsoft Silverlight 5” framework installed, the user will be redirected to a web page on Microsoft.com that offers to install Silverlight on the client machine. This is a less than 7 MB download and should install in a couple of seconds.

7.3 Program overview

The “Gasmetering” application uses input consisting of

- Metering station template (the general type of instruments and layout of these)
- Process conditions, including the actual gas composition
- Properties for the different equipment included in the template

From this input the application then can

1. Compute and visualize the resulting uncertainty in flow measurement values
2. Compute additional relevant properties of the gas composition and process conditions
3. Generate a report and print the report
4. Save work in a file for future use and reference

The following sections describe the functionality in more detail and uses screenshots from the application to illustrate.

7.3.1 Specify metering station template

The start page of the application (Figure 7.1) is also the page where the user specifies the metering station template, meaning the general type of instruments and the layout of these. There are three aspects of the metering station that is modeled:

- **Flow Metering:** what type of meter is used (Orifice, Ultrasonic or Coriolis) and in what configuration (Single Meter, Dual Meter in Series or Dual Meter in Parallel).
- **Line Conditions:** what configuration of sensors is used to measure the line temperature, line pressure and optionally for some templates, line density.
- **Gas Analysis:** how is the gas composition known (by using a Fixed Composition, by Online GC or by Sampling).

By specifying choices for each of these aspects the user is in effect selecting a metering station template. When the user then presses the “Accept and Continue”-button a copy of the selected template is created and the application moves to the first of several input pages, “Conditions” (Figure 7.3). A page navigation menu below the application header is also displayed, where the user now can move freely between different pages (Figure 7.4), some related to input and others related to computed results and visualizations. The pages typically organize content in several sections, and the user can select a section with some form of navigation control.

The selected metering station template is set up with default values, so the user can explore the application functionality without first finish all the data input.

The following pages are available after the metering station template has been selected:

- **Metering Station:** start page where the selected template is displayed. The user can also create a new or open an existing from a file.
- **Conditions:** input regarding flow rate, line conditions and also known gas composition.
- **Gas Analysis:** input regarding uncertainty in known gas composition.
- **Flow Measurement:** input regarding uncertainty in instrumentation and other facilities used for flow measurement (for example flow calibration).
- **Results:** computed uncertainty of the main flow measurement variables (standard volume flow, mass flow and energy flow) displayed as uncertainty budgets tables.
- **Charts:** computed uncertainty of the main flow measurement variables (standard volume flow, mass flow and energy flow) and some other essential equipment, displayed as uncertainty budgets charts.
- **Plots:** computed uncertainty of the main flow measurement variables (standard volume flow, mass flow and energy flow) as function of a selected flow rate range, displayed as plots.
- **Report:** summary of the uncertainty analysis formatted as an on-screen report. This can be printed, and it is also possible to save the analysis in an encrypted file for later use and reference.

The user can move between the input pages in any order, but due to computational dependencies the following work flow is recommended when input data: “Conditions”->”Gas Analysis”->”Flow Measurement”. Also, the logical flow between sections in each page is typically from left to right.

Regarding metering station template, note that when specifying dual flow meters in series or parallel (Figure 7.2), there will be an option to select whether the laboratory flow calibration is performed on both flow meters at the same time. If this is the case it introduces a correlation that the application is able to model.

The following discusses each of the pages.

Figure 7.1 *Gasmetering application start page, where the user specifies the metering station template. It is also possible to open a previously saved file.*

Flow Metering

Single Meter
Dual in Series
☒ Dual in Parallel

Ultrasonic

Line Conditions

Temperature: Average
Pressure: Average
Densitometer: Average
Dens. Type: HasTempAndPress

Gas Analysis

Gas Composition From: FixedComposition

☒ Flow meters calibrated at the same time and location

Accept and Continue Open From File..

Figure 7.2 Metering station with dual ultrasonic flow meters in parallel and also dual line condition instrumentation. Note the “Flow Calibrations calibrated at the same time and location”-check box in the lower left corner. This specifies whether the laboratory flow calibration is performed on both flow meters at the same time.

ABOUT NFOGM NORSK FORRENING FOR OLJIE OG GASSMÅLING OLJEDIREKTORATET Tekna cmr NFOGM v1.2 propose improvements

Fiscal Gas Metering Station Uncertainty

metering station conditions gas analysis flow meas results charts plots report

Process Conditions

Input tables for specifying process conditions that will be used in the uncertainty calculations. The conditions can be changed later. Values in blue color can be edited, and the most significant values are in bold. For efficient input, use TAB key to move to next cell.

LINE CONDITIONS GAS COMPOSITION

Flow Rate: 100000 ☒ Sm³/h ☐ kg/h ☐ GJ/h

Meter Line Operating Conditions				
Line pressure	P	100	bara	
Line temperature	T	50	°C	
Ambient (air) temperature	Tair	0	°C	<input checked="" type="checkbox"/> Use default (0)

Densitometer Line Operating Conditions				
Temperature at densitometer	Td	50	°C	<input checked="" type="checkbox"/> Use default (Line temperature, T)

Additional Operating Conditions				
Viscosity	μ	1.05E-05	Ns/m ²	<input checked="" type="checkbox"/> Use default (1.05E-5)

Figure 7.3 “Conditions”-page and “Line Conditions”-section, where the user specifies the line operating conditions.

metering station conditions gas analysis flow meas results charts plots report

Figure 7.4 Page navigation menu where the user can move freely between different pages, some related to input and others related to computed results and visualizations.

7.3.2 Conditions Page

There are two aspects of the process conditions that the application can model, and these have separate sections in the page:

- **Line Conditions:** includes the flow rate, line pressure and line temperature, and depending on the template selected some other conditions.
- **Gas Composition:** consist of gas component concentration values (mole %) of a fixed set of known components (Figure 7.5).

Regarding “Line Conditions” note that some of the parameters may have default values that can be activated. Default values can be constant numbers or can be computed from other parameters (Figure 7.3).

Regarding “Gas Composition” (Figure 7.5), note that a set of gas properties for the specified composition is computed according to AGA 8, AGA 10 and ISO 6976. These are used later in model computations and are in addition displayed here for convenience.

metering station conditions gas analysis flow meas results charts plots report

Process Conditions

Input tables for specifying process conditions that will be used in the uncertainty calculations. The conditions can be changed later. Values in blue color can be edited, and the most significant values are in bold. For efficient input, use TAB key to move to next cell.

LINE CONDITIONS					GAS COMPOSITION				
Gas Components					Computed Gas Properties (AGA8, AGA10, ISO6976)				
Methane	C1	86.29	86.29	mole %	Compressibility at line conditions	Z	0.83487		
Ethane	C2	6.01	6.01	mole %	Compressibility at std. ref. conditions	Z _e	0.99704		
Propane	C3	3	3	mole %	Gas Density at line conditions	ρ	86.37582	kg/m ³	
iso-Butane	iC4	1.1	1.1	mole %	Gas Density at std. ref. conditions	ρ _e	0.82186	kg/m ³	
n-Butane	nC4	0.9	0.9	mole %	Molar mass	m	19.37539	g/mol	
iso-Pentane	iC5	0.35	0.35	mole %	Isentropic exponent	κ	1.41095		
n-Pentane	nC5	0.25	0.25	mole %	Velocity of sound	c	404.16569	m/s	
Hexane	C6	0.1	0.1	mole %	Super. calorific value, 25°C Exhaust	H _s	52.21722	MJ/kg	
Heptane	C7	0	0	mole %	Super. calorific value, 25°C Exhaust	H _s	42.91546	MJ/Sm ³	
Octane	C8	0	0	mole %	Infer. calorific value, 25°C Exhaust	H _i	47.28966	MJ/kg	
Nonane	C9	0	0	mole %	Infer. calorific value, 25°C Exhaust	H _i	38.86567	MJ/Sm ³	
Decane	C10	0	0	mole %	CO ₂ Emission Factor	C _m	2.72368	kg/kg	
Nitrogen	N2	1	1	mole %	CO ₂ Emission Factor	C _v	2.23850	kg/Sm ³	
Carbon Dioxide	CO2	1	1	mole %	CO ₂ Emission Factor	C _e	57.59569	tonnes/TJ	
Water	H2O	0	0	mole %					
Hydrogen Sulphide	H2S	0	0	mole %					
Hydrogen	H2	0	0	mole %					
Carbon Monoxide	CO	0	0	mole %					
Oxygen	O2	0	0	mole %					
Helium	He	0	0	mole %					
Argon	Ar	0	0	mole %					

Figure 7.5 “Conditions”-page and “Gas Composition”-section, where the user specifies the gas composition.

When “Sampling” is chosen for “Gas Analysis” in the template the user can enter the samples in a table, or import the data from an Excel CSV file as seen in Figure 7.6. An average composition will be computed as displayed in the “Gas Composition” section and used further in the computation. There will also be an uncertainty contribution modeled by “student-t”-distribution in the uncertainty calculation of the gas analysis (as seen in the section “Sampling Gas Samples” on the “Gas Analysis”-page for this template).

metering station conditions gas analysis flow meas results charts plots report

Process Conditions

Input tables for specifying process conditions that will be used in the uncertainty calculations. The conditions can be changed later. Values in blue color can be edited, and the most significant values are in bold. For efficient input, use TAB key to move to next cell.

LINE CONDITIONS

GAS SAMPLING

GAS COMPOSITION

Add Sample

Delete Last Sample

Import Excel CSV File..

CSV format: one line per sample, no headers, values format 1,0;2,0;3,0;
All values in mol %

#	C1	C2	C3	iC4	nC4	iC5	nC5	C6	C7	C8	C9	C10	N2	CO2	H2O	H2S	H	CO	O2	He	Ar
1	86.29	6.01	3	1.1	0.9	0.35	0.25	0.1	0	0	0	0	1	1	0	0	0	0	0	0	0
2	86.29	6.01	3	1.1	0.9	0.35	0.25	0.1	0	0	0	0	1	1	0	0	0	0	0	0	0
3	86.29	6.01	3	1.1	0.9	0.35	0.25	0.1	0	0	0	0	1	1	0	0	0	0	0	0	0
4	86.29	6.01	3	1.1	0.9	0.35	0.25	0.1	0	0	0	0	1	1	0	0	0	0	0	0	0
5	86.29	6.01	3	1.1	0.9	0.35	0.25	0.1	0	0	0	0	1	1	0	0	0	0	0	0	0
6	86.29	6.01	3	1.1	0.9	0.35	0.25	0.1	0	0	0	0	1	1	0	0	0	0	0	0	0
7	86.29	6.01	3	1.1	0.9	0.35	0.25	0.1	0	0	0	0	1	1	0	0	0	0	0	0	0

Figure 7.6 “Conditions”-page and “Gas Sampling”-section. This section is available when “Sampling” is chosen for “Gas Analysis” in the template. The user can enter the samples in a table, or import the data from an Excel CSV file.

7.3.3 Gas Analysis Page

The gas analysis page encompasses uncertainty in the known gas composition. The details of the specification depend on the type of gas analysis that has been performed. Figure 7.7 shows the input layout if “Sampling” (with GC) has been used, and it is also possible to choose different levels of details in the specification. The page will always include a section “Gas Properties” (Figure 7.8). This contains computed uncertainties of some important factors used in the models of the flow measurement uncertainties and listed here for user convenience. In addition, the section contains user controls for selecting model standards for Z (AGA 8 or user defined) and Z_0 (AGA 8, ISO 6976 or user defined).

The different choices for gas analysis uncertainty are as follows:

- **Fixed Composition**
 - Specify uncertainty in component using mol %, 95% conf.
- **Online GC**
 - Overall Input Level: Select standard for overall uncertainty
 - ASTM D1945, Section 10.1.1
 - NORSOK I-104, Section 9.1.4.1 (under the heading “Fiscal gas composition”)
 - NORSOK I-106, Section 12.2.6.2.8
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)
 - Detailed: Select standard for calibration and repeatability
 - Calibration gas:
 - NORSOK I-104, Section 9.1.4.1
 - NORSOK I-106, Section 12.2.6.2.1

- 1 %: Relative expanded uncertainty with 95 % confidence level of each gas component is 1 % (meaning that if e.g. molar fraction of a gas component is 10 %, the absolute expanded uncertainty of that molar fraction is 0.1 % (abs), corresponding to 1 % of the molar fraction of 10 %).
 - 2%: Relative expanded uncertainty with 95 % confidence level of each gas component is 2 %
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)
 - Repeatability:
 - NORSOK I-104, Section 9.1.4.1
 - NORSOK I-106, Section 12.2.6.2.2
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)
 - Linearity:
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)
- **Sampling**
 - GC analysis
 - Overall Input Level: Select standard for overall uncertainty
 - ASTM D1945, Section 10.1.1
 - NORSOK I-104, Section 9.1.4.1 (under the heading “Fiscal gas composition”)
 - NORSOK I-106, Section 12.2.6.2.8
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)
 - Detailed: Select standard for calibration and repeatability
 - Calibration gas:
 - NORSOK I-104, Section 9.1.4.1
 - NORSOK I-106, Section 12.2.6.2.1
 - 1 %: Relative expanded uncertainty with 95 % confidence level of each gas component is 1 % (meaning that if e.g. molar fraction of a gas component is 10 %, the absolute expanded uncertainty of that molar fraction is 0.1 % (abs), corresponding to 1 % of the molar fraction of 10 %).
 - 2%: Relative expanded uncertainty with 95 % confidence level of each gas component is 2 %
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)
 - Repeatability:
 - NORSOK I-104, Section 9.1.4.1
 - NORSOK I-106, Section 12.2.6.2.2
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)
 - Linearity:
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)

metering station conditions gas analysis flow meas results charts plots report

Gas Analysis Properties and Uncertainty Specification

Input forms for specifying properties and uncertainties of the gas analysis equipment in the metering station. Values in blue color can be edited. For efficient input, use TAB key to move to next cell.

GC ANALYSIS

SAMPLING GAS SAMPLES

GAS PROPERTIES

Overall Input Level ☐

Select standards for calibration and repeatability: NORSOK I104 NORSOK I104

Component		Concentration mol%	Calibration Gas mol %, 95% Conf.	Repeatability mol%, 95% Conf.	Linearity mol%, 95% Conf.	Total Unc. mol%, 95% Conf.	Relative Unc. %
Methane	C1	86.29	0.1726	0.1	0	0.1995	0.23
Ethane	C2	6.01	0.0301	0.04	0	0.05	0.83
Propane	C3	3	0.015	0.04	0	0.0427	1.42
iso-Butane	iC4	1.1	0.0055	0.04	0	0.0404	3.67
n-Butane	nC4	0.9	0.009	0.04	0	0.041	4.56
iso-Pentane	iC5	0.35	0.0035	0.04	0	0.0402	11.47
n-Pentane	nC5	0.25	0.0025	0.04	0	0.0401	16.03
Hexane	C6	0.1	0.005	0.04	0	0.0403	40.31
Heptane	C7	0	0	0	0	0	0
Octane	C8	0	0	0	0	0	0
Nonane	C9	0	0	0	0	0	0
Decane	C10	0	0	0	0	0	0
Nitrogen	N2	1	0.005	0.04	0	0.0403	4.03
Carbon Dioxide	CO2	1	0.005	0.04	0	0.0403	4.03

Figure 7.7 Input of uncertainties for gas analysis when “sampling” (with GC) is selected.

metering station conditions gas analysis flow meas results charts plots report

Gas Analysis Properties and Uncertainty Specification

Input forms for specifying properties and uncertainties of the gas analysis equipment in the metering station. Values in blue color can be edited. For efficient input, use TAB key to move to next cell.

GC ANALYSIS
GAS PROPERTIES

Select Z_0 and Z specification to be used for uncertainty calculation of gas properties dependent on compressibility

Z₀ Specification: ☒ ISO 6976 ☐ AGA8 ☐ User Def. [% , 95% conf.] 0.0522
Z Specification: ☒ AGA8 ☐ User Def. [% , 95% conf.] 0.1

Uncertainty in CO2 Emission Factors and Calorific Value			
CO2 Emission Factor in kg/kg	0.182	%	95 % Confidence
CO2 Emission Factor in kg/Sm ³	0.317	%	95 % Confidence
CO2 Emission Factor in tonnes/TJ	0.081	%	95 % Confidence
Sup. Calorific Value in MJ/kg	0.216	%	95 % Confidence
Inf. Calorific Value in MJ/kg	0.431	%	95 % Confidence

Standard Volume Flow Model: uncertainty in Z_0/\sqrt{mZ} factor due to model, line conditions and gas composition uncertainties

Input Variable	Uncertainty	Unit	Confidence	Std. Uncert. u_i	Sens. Coeff. s_i	Variance ($s_i \cdot u_i$) ²
Z_0 ,mod	0.0522	%	95% (norm)	0.0261 %	1.000 e+0	6.812 e-4 (%) ²
Zmod	0.1	%	95% (norm)	0.05 %	5.000 e-1	6.250 e-4 (%) ²
Z_0/\sqrt{mZ} ,ana	0.0973	%	95% (norm)	0.0487 %	1.000 e+0	2.368 e-3 (%) ²

Sum of variances, $\sum (s_i \cdot u_i)^2$
0.0037 (%)²

Relative Combined Standard Uncertainty
0.061 %

Relative Expanded Uncertainty (95% Confidence level, k=2)
0.121 %

Figure 7.8 Computed uncertainties of some important factors used in the models of the flow measurement uncertainties. In addition, the section contains user controls for selecting model standards for Z and Z_0 .

7.3.4 Flow Measurement Page

The flow measurement page encompasses specification of uncertainty in instruments and other facilities used for flow measurement (Figure 7.9). Simple instruments like a temperature transmitter has one section for uncertainty specification, but more complex instruments like an orifice flow meter have several sections (as can be seen in Figure 7.9). Some instruments also include flow calibration data (Figure 7.10). Note that it can be selected how the meter is adjusted for the calibration curve, as described in Appendix A.

Depending on the equipment there can be functionality for using values from different standard specifications, as shown in Figure 7.9 where the user can select “ISO 5167 Specification” for the uncertainty in the orifice meter pipe diameter. An overall level can also be selected as the total uncertainty may depend on design, operational and maintenance routines designed to keep measurements within a given maximum uncertainty. The uncertainty requirements in the Norwegian measurement regulations has been pre entered as default values. There can also be functionality for storing frequently used specifications in files for later retrieval, as shown in Figure 7.11 where the detailed input for a temperature transmitter is shown. The “Save”-button can be used to save the complete specification to a file, and the “Load”-button can then later be used for quickly loading the saved specification for a temperature transmitter.

ABOUT NFOGM NORSE FORMING FOR OIL AND GAS MEASURING OLJEDIREKTORATET Tekna cmr INFOGM v1.2 propose improvements

Fiscal Gas Metering Station Uncertainty

metering station conditions gas analysis flow meas results charts plots report

Flow Measurement Properties and Uncertainty Specification

Input forms for specifying properties and uncertainties of the flow meter equipment in the metering station. Values in blue color can be edited. Data for common equipment can be stored in template files and later be recalled. For efficient input, use TAB key to move to next cell.

ORIFICE METER PIPE DIAMETER ORIFICE METER ORIFICE DIAMETER ORIFICE METER DISCHARGE COEFF. ORIFICE METER DIFF. PRESSURE LINE CONDITIONS TEMPERATURE LINE CONDITIONS PRESSURE LINE CONDITIO DENSITOMET

ISO 5167 Specification ☒

Properties and Constants

Pipe Diameter 300 mm

Input Variable	Uncertainty	Unit	Confidence	Std. Uncert. u_i	Sens. Coeff. s_i	Variance $(s_i \cdot u_i)^2$
Uncertainty	0.4	%	95% (norm)	0,6 mm	1,000 e+0	3,600 e-1 (mm) ²

Combined Standard Uncertainty, U_c 0,6 mm

Expanded Uncertainty (95% Confidence level, $k=2$), $k \cdot U_c$ 1,2 mm

Value 300 mm

Relative Expanded Uncertainty (95% Confidence level, $k=2$) 0,4 %

0.4 % according to ISO 5167 Part 2 chapter 5.3.3.2

Figure 7.9 Flow measurement page for a template with orifice flow meter.

FLOW METER LAB CALIBRATION FLOW METER FIELD UNCERTAINTY LINE CONDITIONS TEMPERATURE LINE CONDITIONS PRESSURE LINE CONDITIONS DENSITOMETER DENSITOMETER TEMPERATURE

Properties and Constants

Line pressure at cal. 50 bara

Line temperature at cal. 10 °C

Add Calibration Point Remove Last Point Correction for deviation: ☒ None ☐ Linear Interpolation ☐ Flow Independent [%] 0

#	Rate m ³ /h	Deviation (Uncorrected) %	Lab. Reference %, 95% Conf.	Repeatability %, 95% Conf.	Total %, 95% Conf.
1	107	1.2	0.2	0.1	1.3873
2	267	0.55	0.2	0.1	0.67
3	668	0.3	0.2	0.1	0.4114
4	1069	0.23	0.2	0.1	0.3467
5	1871	0.18	0.2	0.1	0.305
6	2673	0.2	0.2	0.1	0.3211
7	3475	0.24	0.2	0.1	0.3556

Figure 7.10 Flow measurement page for a template with ultrasonic flow meter. Note that the method for adjusting (correcting) the flow meter after calibration is to be specified here. See also Appendix A.

FLOW METER
LAB CALIBRATION

FLOW METER
FIELD UNCERTAINTY

LINE CONDITIONS
TEMPERATURE

LINE CONDITIONS
PRESSURE

LINE CONDITIONS
DENSITOMETER

DENSITOMETER
TEMPERATURE

Overall Input Level ☐

Load ..

Save ..

Properties and Constants

Time Between Calibrations

12

Months

Ambient Temp. At Calibration

20

°C

Input Variable	Uncertainty	Unit	Confidence	Std. Uncert. u_i	Sens. Coeff. s_i	Variance $(s_i \cdot u_i)^2$
Temp. elem. and transm.	0.1	°C	99% (norm)	0,0333 °C	1,000 e+0	1,111 e-3 (°C) ²
Stability	0.1	%MV/24mc	99% (norm)	0,0539 °C	1,000 e+0	2,901 e-3 (°C) ²
RFI Effects	0.1	°C	99% (norm)	0,0333 °C	1,000 e+0	1,111 e-3 (°C) ²
Ambient temp. effect	0.0015	°C/°C	99% (norm)	0,01 °C	1,000 e+0	1,000 e-4 (°C) ²
Stability - temp. element	0.05	°C	95% (norm)	0,025 °C	1,000 e+0	6,250 e-4 (°C) ²
Misc.	0	°C	95% (norm)	0 °C	1,000 e+0	0,000 e+0 (°C) ²

Sum of variances, $U_c^2 = \sum (s_i \cdot u_i)^2$

5,848 e-3 (°C)²

Combined Standard Uncertainty, U_c

0,076 °C

Expanded Uncertainty (95% Confidence level, $k=2$), $k \cdot U_c$

0,153 °C

Value

50 °C

Relative Expanded Uncertainty (95% Confidence level, $k=2$)

0,047 %

Ref. Norwegian Petroleum Directorate Measurement Regulation; Measurement regulation §8; Circuit uncertainty limits.

Figure 7.11 Detailed input for a temperature transmitter. The “Save”-button can be used to save the complete specification to a file, and the “Load”-button can then later be used for quickly loading the saved specification.

7.3.5 Uncertainty Calculation Results Page

This page is the first of several pages that displays the result of the uncertainty calculation based on the input data (Figure 7.12). There is one section for each of the main flow measurement variables, standard volume flow, mass flow and energy flow. Depending on template there can be sections for additional measurements. For example, if the template included ultrasonic flow meter together with using GC for gas analysis, there is a section for the density measurement.

The uncertainty is displayed as uncertainty budgets tables, and the functional relationship is displayed for reference. Depending on the selected metering template, there can also be a list of “computed values”. These are values computed from the input data for use in the uncertainty calculation and listed here for convenience.

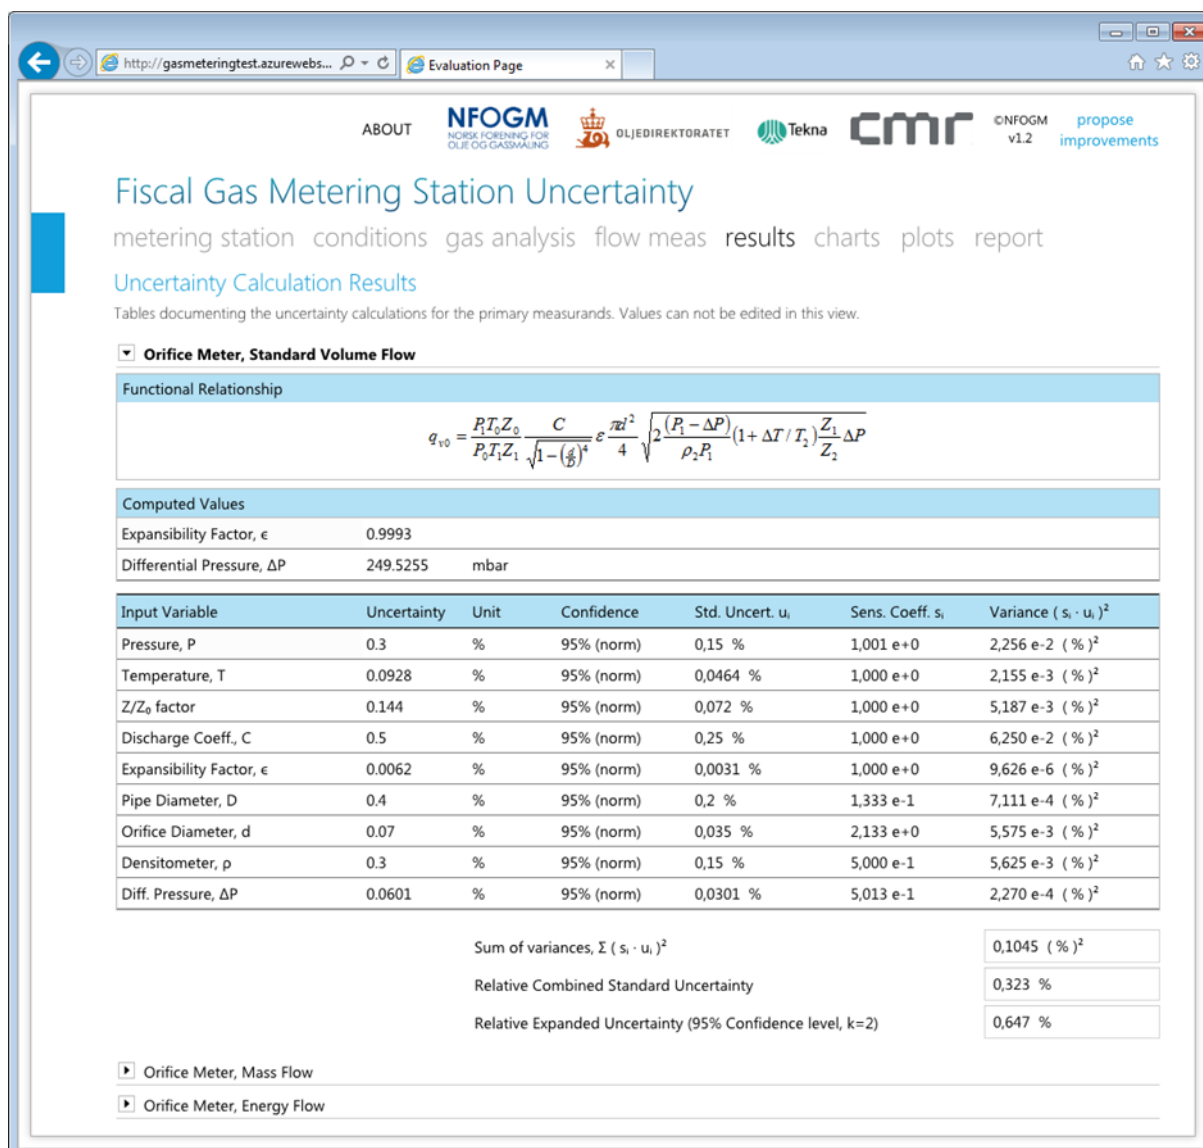


Figure 7.12 Computed uncertainty of the main flow measurement variables (standard volume flow, mass flow and energy flow) displayed as uncertainty budgets tables.

7.3.6 Uncertainty Budget Charts Page

This page displays the computed uncertainty of the main flow measurement variables (standard volume flow, mass flow and energy flow) displayed as uncertainty budgets charts (Figure 7.13). Depending on template it also contains charts for other essential equipment, for example temperature and pressure transmitters (Figure 7.13). The bar chart displays numerical values when the mouse pointer hover over a bar, and the "Export Image"-button let the user save an image of the chart to a file.



Figure 7.13 Computed uncertainty of the main flow measurement variables and equipment displayed as uncertainty budgets charts.

7.3.7 Uncertainty Range Plots Page

This page contains computed uncertainty of the main flow measurement variables (standard volume flow, mass flow and energy flow) as function of a selected flow rate range, displayed as plots (Figure 7.14). It is possible to select the flow rate range, and also the flow rate unit (Sm^3/h , kg/h , GJ/h). Numerical values are displayed when the mouse pointer hover over a point, and the “Export Image”-button let the user save an image of the plot to a file.

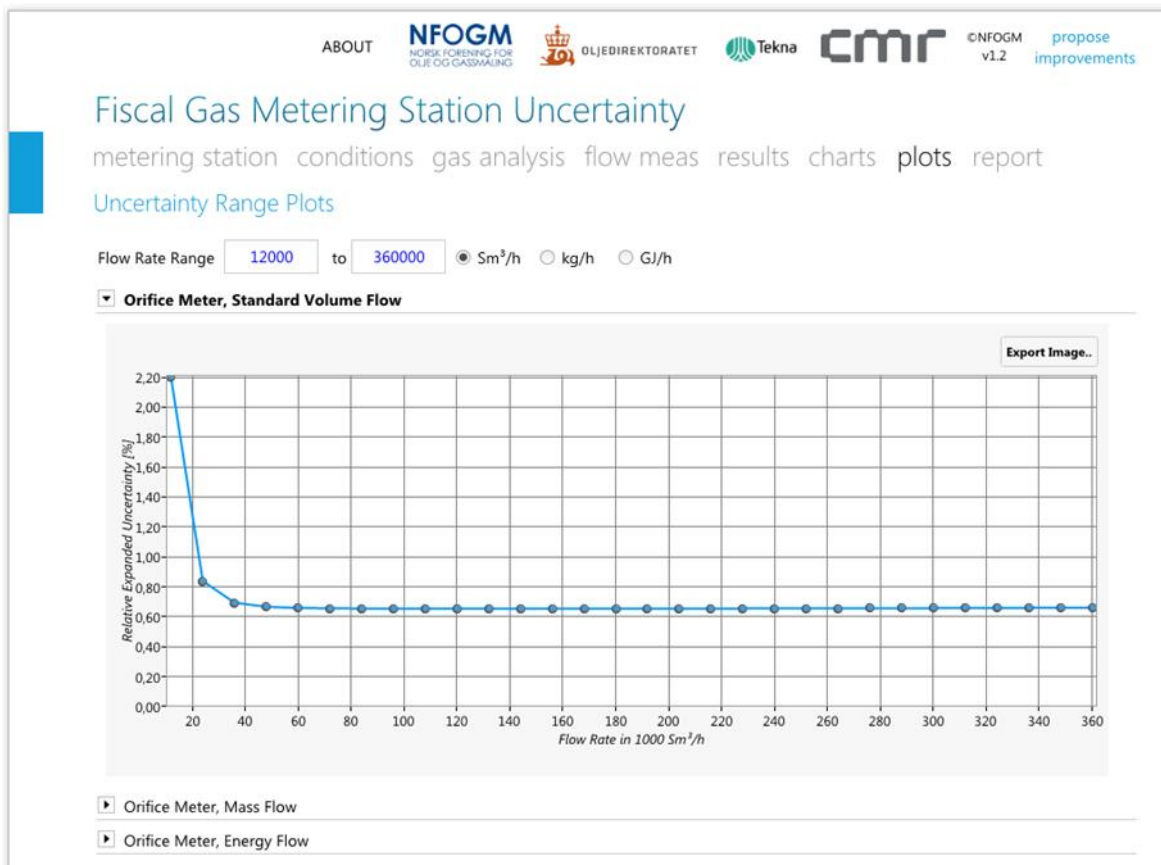


Figure 7.14 Computed uncertainty of the main flow measurement variables plotted over a selectable flow range.

7.3.8 Uncertainty Report Page

This page contains a summary of the uncertainty analysis formatted as an on-screen report (Figure 7.15). This can be printed, and it is also possible to save the analysis in an encrypted file for later use and reference. Regarding printing, note that it is possible to “print to pdf file” by installing an appropriate printer driver. “Adobe Acrobat” includes a printer driver with this functionality, and “PDFCreator” is another (free) alternative.

The report includes the following:

- Header which integrates the <Name>, <Date> and <Description> input from start page.
- Graphic that displays the selected metering station template.
- Tables listing the line operating conditions.
- Table listing the computed gas properties according to AGA 8, AGA 10 and ISO 6976.

- Uncertainty budget for standard volume flow at the given flow rate in units of Sm^3/h . The functional relationship is displayed together with any relevant computed values used in the model.
- Uncertainty budget for mass flow at the given flow rate in units of kg/h . The functional relationship is displayed together with any relevant computed values used in the model.
- Uncertainty budget for energy flow at the given flow rate in units of GJ/h . The functional relationship is displayed together with any relevant computed values used in the model.
- Uncertainty budget for additional measurements, depending on template. For example, if the template included ultrasonic flow meter together with using GC for gas analysis, there is an uncertainty budget for the density measurement.
- Uncertainty in CO_2 emission factors and calorific value.

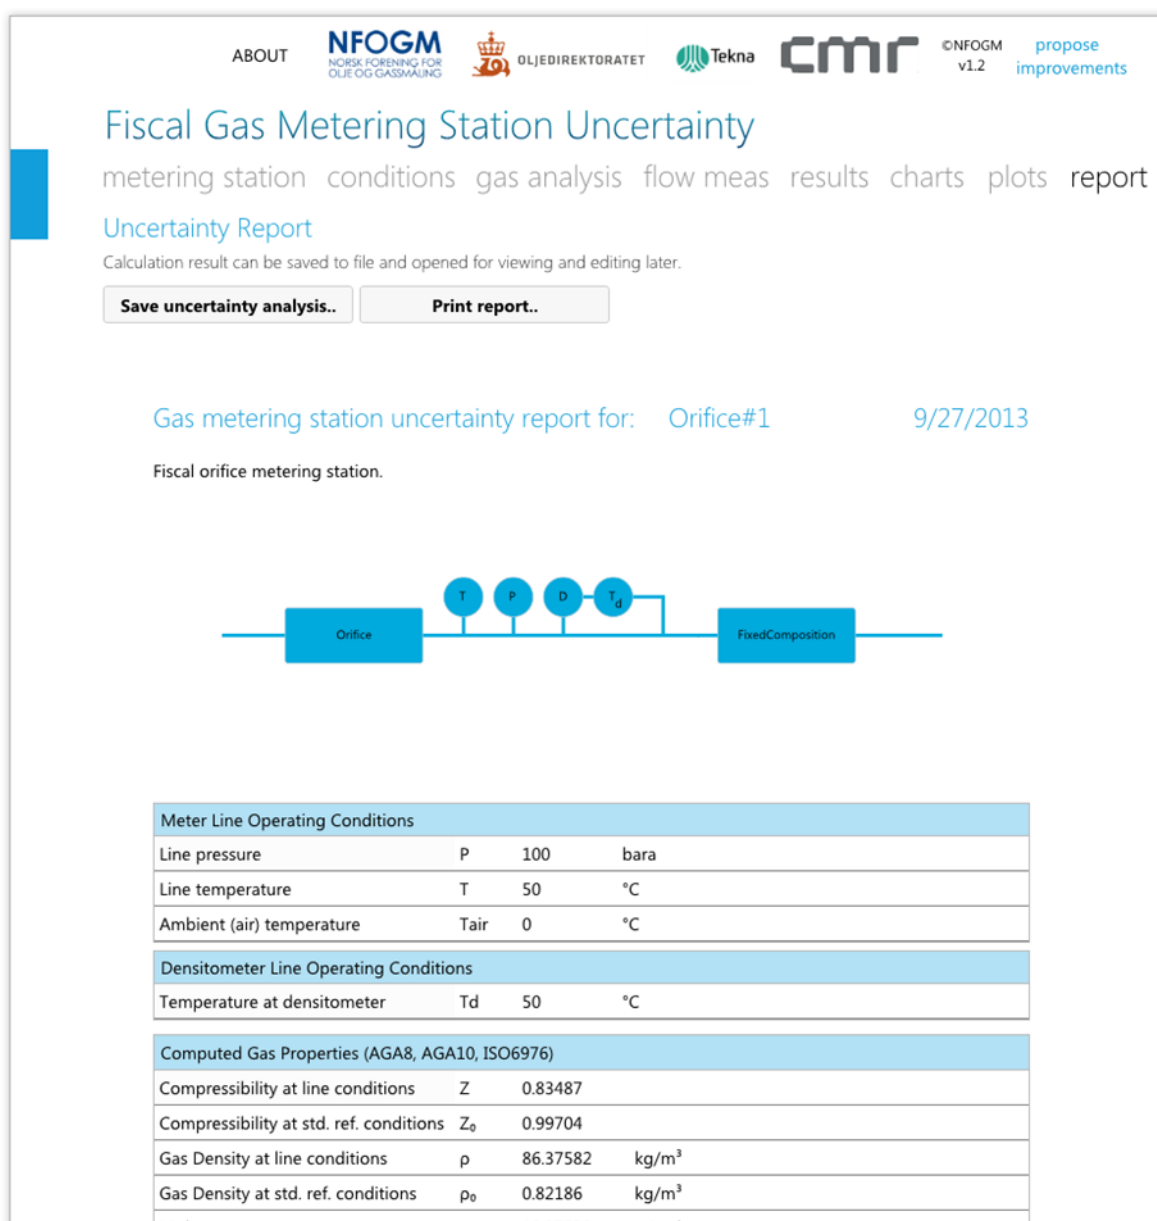


Figure 7.15 Report page contains a summary of the uncertainty analysis formatted as an on-screen report. This can be printed, and it is also possible to save the analysis in an encrypted file for later use and reference.

7.3.9 Note about “Save” and “Open” functionality

When the user saves an uncertainty analysis to file, it will always be a new file. It is not possible to save “changes” to an existing file. In practice this is not a limitation. If the user opens an uncertainty analysis file and want to “save changes”, it is always possible to just use the same file name and thereby overwrite the file.

While this mechanism seems like an unnecessary limitation, it is in fact an important security feature of Silverlight. A Silverlight application cannot generally access the file system on a computer. The only exception to this is if the user is shown a file select dialog (controlled by the system, not the application) and then selects a specific file to open and read (read-only) or a name for a file to create (write-only). Through the system-controlled file dialog the user has full control over what files the application can read, and over what file areas and file name the application can write to.

7.3.10 Note about “opening” an uncertainty analysis file

When the application start page is first shown the two buttons at the bottom right “Accept and Continue” and “Open From File” is both enabled. If the user chooses either of these the application moves to the “Conditions” page. If the user now goes back to the start page the “Open From File” button is no longer enabled and the “Accept and Continue” button have changed name to “Create New”. It is therefore not possible to open an uncertainty analysis file from this state. To either create a new uncertainty analysis or open an existing from file the user must first press the “Create New” button. This returns the application to the initial state where both the “Accept and Continue” and “Open From File” is enabled.

8 GasMetApp Web Application

This chapter documents the GasMetApp web application for carrying out uncertainty analyses based on the uncertainty models described in this report. It should here be emphasised that this report is a documentation of the uncertainty models and the corresponding web-based calculation tool. Therefore, the example input values in that calculation tool are just examples and should not be regarded as recommended values by NFOGM, NORCE, NPD or any other party.

8.1 Software platform

The new web application was developed in 2020 and is based on the open-source Blazor platform, developed by Microsoft (<https://blazor.net>). This platform only uses open web standards recommended by W3C (<https://www.w3.org/>), including HTML5 and WebAssembly (<https://webassembly.org/>). Since Blazor uses C#, the same language used to implement the original Silverlight application, it has been possible to reuse much of the code.

When the user visits a web page all the files that constitutes the application will be downloaded and the application will run in the browser without need for any further communication with the web server. The application files are stored in the web browser cache and will only be downloaded again if there is a new version available.

The web application is supported on all web browsers that supports WebAssembly 1.0 or later, and this includes all major browsers on both Windows, Linux, Mac and also mobile and other operating systems (<https://caniuse.com/#feat=wasm>). Note that Internet Explorer 11 does not support WebAssembly and cannot be used to run the new web application.

8.2 Installation and use

The web address for the application will be published on nfogm.no. By visiting the published address, all the files that constitutes the application will be downloaded and the application will run in the browser without need for any further communication with the web server. The application files are stored in the web browser cache and will only be downloaded again if there is a new version available.

8.3 Program overview

The application uses input consisting of

- Metering station template (the general type of instruments and layout of these)
- Process conditions, including the actual gas composition
- Properties for the different equipment included in the template

From this input the application then can

1. Compute and visualize the resulting uncertainty in flow measurement values
2. Compute additional relevant properties of the gas composition and process conditions
3. Generate a report and print the report
4. Save work in a file for future use and reference

The following sections describe the functionality in more detail and uses screenshots from the application to illustrate.

8.3.1 Specify metering station template

The start page of the application (Figure 8.1) is also the page where the user specifies the metering station template, meaning the general type of instruments and the layout of these. There are three aspects of the metering station that is modeled:

- **Flow Metering:** what type of meter is used (Orifice, Ultrasonic or Coriolis) and in what configuration (Single Meter, Dual Meter in Series or Dual Meter in Parallel).
- **Line Conditions:** what configuration of sensors is used to measure the line temperature, line pressure and optionally for some templates, line density.
- **Gas Analysis:** how is the gas composition known (by using a Fixed Composition, by Online GC or by Sampling).

By specifying choices for each of these aspects the user is in effect selecting a metering station template. When the user then presses the "Accept and Continue"-button a copy of the selected template is created and the application moves to the first of several input pages, "Conditions" (Figure 8.3). A page navigation menu below the application header is also displayed, where the user now can move freely between different pages (Figure 8.4), some related to input and others related to computed results and visualizations. The pages typically organize content in several sections, and the user can select a section with some form of navigation control.

The selected metering station template is set up with default values, so the user can explore the application functionality without first finish all the data input.

The following pages are available after the metering station template has been selected:

- **Metering Station:** start page where the selected template is displayed. The user can also create a new or open an existing from a file.
- **Conditions:** input regarding flow rate, line conditions and also known gas composition.
- **Gas Analysis:** input regarding uncertainty in known gas composition.
- **Flow Measurement:** input regarding uncertainty in instrumentation and other facilities used for flow measurement (for example flow calibration).
- **Results:** computed uncertainty of the main flow measurement variables (standard volume flow, mass flow and energy flow) displayed as uncertainty budgets tables.
- **Charts:** computed uncertainty of the main flow measurement variables (standard volume flow, mass flow and energy flow) and some other essential equipment, displayed as uncertainty budgets charts.
- **Report:** summary of the uncertainty analysis formatted as an on-screen report. This can be printed, and it is also possible to save the analysis in an encrypted file for later use and reference.


The user can move between the input pages in any order, but due to computational dependencies the following work flow is recommended when input data: "Conditions"->"Gas Analysis"->"Flow Measurement". Also, the logical flow between sections in each page is typically from left to right.

Regarding metering station template, note that when specifying dual flow meters in series or parallel (Figure 8.2), there will be an option to select whether the laboratory flow calibration is performed on both flow meters at the same time. If this is the case it introduces a correlation that the application is able to model.

The following discusses each of the pages.

Figure 8.1 *GasMetApp application start page, where the user specifies the metering station template. It is also possible to open a previously saved file.*

Figure 8.2 *Metering station with dual ultrasonic flow meters in parallel and also dual line condition instrumentation. Note the “Flow Calibrations calibrated at the same time and location”-check box in the lower left corner. This specifies whether the laboratory flow calibration is performed on both flow meters at the same time.*

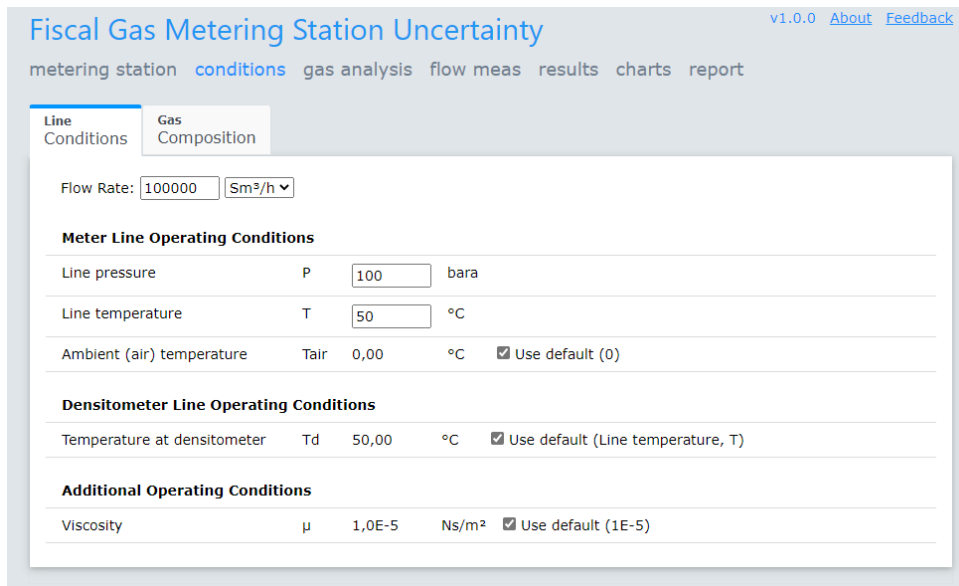

Fiscal Gas Metering Station Uncertainty v1.0.0 [About](#) [Feedback](#)

metering station **conditions** gas analysis flow meas results charts report

Line Conditions Gas Composition

Flow Rate: 100000 Sm³/h

Meter Line Operating Conditions

Line pressure	P	100	bara
Line temperature	T	50	°C
Ambient (air) temperature	Tair	0,00	°C <input checked="" type="checkbox"/> Use default (0)

Densitometer Line Operating Conditions

Temperature at densitometer	Td	50,00	°C <input checked="" type="checkbox"/> Use default (Line temperature, T)
-----------------------------	----	-------	--

Additional Operating Conditions

Viscosity	μ	1,0E-5	Ns/m ² <input checked="" type="checkbox"/> Use default (1E-5)
-----------	---	--------	--

Figure 8.3 “Conditions”-page and “Line Conditions”-section, where the user specifies the line operating conditions.




Figure 8.4 Page navigation menu where the user can move freely between different pages, some related to input and others related to computed results and visualizations.

8.3.2 Conditions Page

There are two aspects of the process conditions that the application can model, and these have separate sections in the page:

- **Line Conditions:** includes the flow rate, line pressure and line temperature, and depending on the template selected some other conditions.
- **Gas Composition:** consist of gas component concentration values (mole %) of a fixed set of known components (Figure 8.5).

Regarding “Line Conditions” note that some of the parameters may have default values that can be activated. Default values can be constant numbers or can be computed from other parameters (Figure 8.3).

Regarding “Gas Composition” (Figure 8.5), note that a set of gas properties for the specified composition is computed according to AGA 8, AGA 10 and ISO 6976. These are used later in model computations and are in addition displayed here for convenience.

Fiscal Gas Metering Station Uncertainty v1.0.0 [About](#) [Feedback](#)

metering station [conditions](#) gas analysis flow meas results charts report

Line Conditions

Gas Composition

Name	Symbol	Conc	NormConc	Unit
Methane	C1	86,29	86,29	mole %
Ethane	C2	6,01	6,01	mole %
Propane	C3	3	3,00	mole %
iso-Butane	iC4	1,1	1,10	mole %
n-Butane	nC4	0,9	0,90	mole %
iso-Pentane	iC5	0,35	0,35	mole %
n-Pentane	nC5	0,25	0,25	mole %
Hexane	C6	0,1	0,10	mole %
Heptane	C7	0	0,00	mole %
Octane	C8	0	0,00	mole %
Nonane	C9	0	0,00	mole %
Decane	C10	0	0,00	mole %
Nitrogen	N2	1	1,00	mole %
Carbon Dioxide	CO2	1	1,00	mole %
Water	H2O	0	0,00	mole %
Hydrogen Sulphide	H2S	0	0,00	mole %
Hydrogen	H2	0	0,00	mole %
Carbon Monoxide	CO	0	0,00	mole %
Oxygen	O2	0	0,00	mole %
Helium	He	0	0,00	mole %
Argon	Ar	0	0,00	mole %

Name	Symbol	Value	Unit
Compressibility at line conditions	Z	0,83487	
Compressibility at std. ref. conditions	Z _o	0,99704	
Gas Density at line conditions	ρ	86,376	kg/m³
Gas Density at std. ref. conditions	ρ _o	0,82186	kg/m³
Molar mass	m	19,375	g/mol
Isentropic exponent	κ	1,4109	
Velocity of sound	c	404,17	m/s
Super. calorific value, 25°C Exhaust	H _s	42,915	MJ/Sm³
Super. calorific value, 25°C Exhaust	H _s	52,217	MJ/kg
Infer. calorific value, 25°C Exhaust	H _i	38,866	MJ/Sm³
Infer. calorific value, 25°C Exhaust	H _i	47,29	MJ/kg
CO ₂ Emission Factor	C _m	2,7237	kg/kg
CO ₂ Emission Factor	C _v	2,2385	kg/Sm³
CO ₂ Emission Factor	C _e	57,596	tonnes/TJ

Figure 8.5 “Conditions”-page and “Gas Composition”-section, where the user specifies the gas composition.

When “Sampling” is chosen for “Gas Analysis” in the template the user can import the data from an Excel CSV file as seen in Figure 8.6. An average composition will be computed as displayed in the “Gas Composition” section (Figure 8.5) and used further in the computation. There will also be an uncertainty contribution modeled by “student-t”-distribution in the uncertainty calculation of the gas analysis (as seen in the section “Sampling Gas Samples” on the “Gas Analysis”-page for this template).

Note that when importing gas samples from a CSV file, these samples will not be added to the existing dataset, but replace it, as suggested by the button name “Use samples from CSV file..”. Also, the “Delete all samples” button will leave one sample left in the dataset, otherwise the gas composition is not defined. The required format of the CSV file is

- No headers
- One line per sample
- Decimal point is “.”
- Value separator is “,”
- Empty cells allowed
- Components in end of list can be omitted if they are all 0
- All values in mol %

For example, the first gas sample in Figure 8.6 can be entered in the CSV file as:

70.08,11.62,9.36,0.84,1.89,0.18,0.17,0.03,,,,,1.03,4.8

It is also possible to copy all or part of the table in Figure 8.6 to Excel as a table. Select range with left mouse button pressed and use standard copy and paste operation into an Excel spreadsheet.

Fiscal Gas Metering Station Uncertainty v1.0.0 [About](#) [Feedback](#)

metering station [conditions](#) [gas analysis](#) [flow meas](#) [results](#) [charts](#) [report](#)

Line Conditions **Gas Sampling** Gas Composition

Use samples from CSV file... Delete all samples Show CSV Example... CSV format: one line per sample, no headers, values format 1.0;2.0;3.0. Empty cells allowed. All values in mol %.

Gas Samples

#	C1	C2	C3	iC4	nC4	iC5	nC5	C6	C7	C8	C9	C10	N2	CO2	H2O	H2S	H	CO	O2	He	Ar
1	70,1	11,6	9,36	0,84	1,89	0,18	0,17	0,03	0	0	0	0	1,03	4,8	0	0	0	0	0	0	0
2	70,1	11,6	9,36	0,84	1,89	0,18	0,17	0,03	0	0	0	0	1,03	4,8	0	0	0	0	0	0	0
3	70,3	11,8	9,05	0,77	1,65	0,12	0,11	0,06	0	0	0	0	1,03	5,17	0	0	0	0	0	0	0
4	68,8	11,7	9,28	0,89	2,13	0,23	0,23	0,06	0	0	0	0	1,2	5,52	0	0	0	0	0	0	0
5	71,5	10,8	8,3	0,79	1,93	0,21	0,2	0,04	0	0	0	0	1,14	5,07	0	0	0	0	0	0	0
6	70,8	11,5	9,06	0,88	2,07	0,23	0,22	0,06	0	0	0	0	0,11	4,99	0	0	0	0	0	0	0
7	69,9	11,6	9,23	0,91	2,12	0,23	0,23	0,06	0	0	0	0	0,99	4,81	0	0	0	0	0	0	0
8	69,6	11,6	9,31	0,93	2,25	0,28	0,28	0,2	0	0	0	0	0,65	4,88	0	0	0	0	0	0	0
9	72,4	11,5	7,77	0,82	1,88	0,24	0,24	0,07	0	0	0	0	0,65	4,43	0	0	0	0	0	0	0
10	72,4	11,1	7,61	0,91	2,29	0,43	0,48	0,26	0	0	0	0	0,44	4,07	0	0	0	0	0	0	0
11	73,6	10,9	7,07	0,79	1,91	0,29	0,32	0,14	0	0	0	0	0,98	4	0	0	0	0	0	0	0
12	73,9	10,8	6,95	0,77	1,82	0,28	0,29	0,12	0	0	0	0	0,9	4,16	0	0	0	0	0	0	0
13	71,7	11,6	8,24	0,83	1,94	0,23	0,22	0,05	0	0	0	0	0,64	4,61	0	0	0	0	0	0	0
14	70,4	11,5	8,58	0,91	2,19	0,28	0,28	0,1	0	0	0	0	0,71	5,05	0	0	0	0	0	0	0
15	71,2	11,3	8,6	0,91	2,24	0,31	0,32	0,08	0	0	0	0	0,51	4,61	0	0	0	0	0	0	0
16	70,9	11,2	8,52	0,9	2,23	0,3	0,32	0,18	0	0	0	0	0,95	4,53	0	0	0	0	0	0	0
17	71,6	11	8,15	0,85	2,1	0,3	0,31	0,18	0	0	0	0	0,68	4,87	0	0	0	0	0	0	0
18	67,7	12,4	9,97	0,91	2	0,21	0,2	0,06	0	0	0	0	0,76	5,77	0	0	0	0	0	0	0
19	68,5	12	9,67	0,9	2,06	0,23	0,24	0,07	0	0	0	0	1	5,32	0	0	0	0	0	0	0
20	67,8	12,3	10,1	0,93	2,1	0,22	0,22	0,06	0	0	0	0	0,9	5,34	0	0	0	0	0	0	0
21	68,2	12,1	9,92	0,9	1,99	0,18	0,16	0,02	0	0	0	0	0,99	5,63	0	0	0	0	0	0	0

Figure 8.6 “Conditions”-page and “Gas Sampling”-section. This section is available when “Sampling” is chosen for “Gas Analysis” in the template. The user can import the data from an Excel CSV file. The expected format of the file is displayed, and the “Show CSV Example..” button will display a dialog with a detailed example.

8.3.3 Gas Analysis Page

The gas analysis page encompasses uncertainty in the known gas composition. The details of the specification depend on the type of gas analysis that has been performed. Figure 8.7 shows the input layout if “Sampling” (with GC) has been used, and it is also possible to choose different levels of details in the specification. The page will always include a section “Gas Properties” (Figure 8.8). This contains computed uncertainties of some important factors used in the models of the flow measurement uncertainties and listed here for user convenience. In addition, the section contains user controls for selecting model standards for Z (AGA 8 or user defined) and Z_0 (AGA 8, ISO 6976 or user defined).

The different choices for gas analysis uncertainty are as follows:

- **Fixed Composition**
 - Specify uncertainty in component using mol %, 95% conf.
- **Online GC**
 - Overall Input Level: Select standard for overall uncertainty
 - ASTM D1945, Section 10.1.1
 - NORSOK I-104, Section 9.1.4.1 (under the heading “Fiscal gas composition”)
 - NORSOK I-106, Section 12.2.6.2.8
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)
 - Detailed: Select standard for calibration and repeatability
 - Calibration gas:
 - NORSOK I-104, Section 9.1.4.1
 - NORSOK I-106, Section 12.2.6.2.1
 - 1 %: Relative expanded uncertainty with 95 % confidence level of each gas component is 1 % (meaning that if e.g. molar fraction of a gas component is 10 %, the absolute expanded uncertainty of that molar fraction is 0.1 % (abs), corresponding to 1 % of the molar fraction of 10 %).
 - 2%: Relative expanded uncertainty with 95 % confidence level of each gas component is 2 %
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)
 - Repeatability:
 - NORSOK I-104, Section 9.1.4.1
 - NORSOK I-106, Section 12.2.6.2.2
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)
 - Linearity:
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)
- **Sampling**
 - GC analysis
 - Overall Input Level: Select standard for overall uncertainty
 - ASTM D1945, Section 10.1.1
 - NORSOK I-104, Section 9.1.4.1 (under the heading “Fiscal gas composition”)
 - NORSOK I-106, Section 12.2.6.2.8

- User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)
- Detailed: Select standard for calibration and repeatability
 - Calibration gas:
 - NORSOK I-104, Section 9.1.4.1
 - NORSOK I-106, Section 12.2.6.2.1
 - 1 %: Relative expanded uncertainty with 95 % confidence level of each gas component is 1 % (meaning that if e.g. molar fraction of a gas component is 10 %, the absolute expanded uncertainty of that molar fraction is 0.1 % (abs), corresponding to 1 % of the molar fraction of 10 %).
 - 2%: Relative expanded uncertainty with 95 % confidence level of each gas component is 2 %
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)
 - Repeatability:
 - NORSOK I-104, Section 9.1.4.1
 - NORSOK I-106, Section 12.2.6.2.2
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)
 - Linearity:
 - User Defined (absolute expanded uncertainty with 95 % confidence level to be given in mole %)

Fiscal Gas Metering Station Uncertainty

v1.0.0 [About](#) [Feedback](#)

metering station
conditions
gas analysis
flow meas
results
charts
report

GC
Analysis

Gas
Properties

☐ Overall Input Level
 Select standard for calibration and repeatability: NORSOK I104 NORSOK I104

Gas Composition

Name	Symbol	Conc mol%	Calibration Gas mol%, 95%	Repeatability mol%, 95%	Linearity mol%, 95%	Total Unc. mol%, 95%	Relative Unc %
Methane	C1	86,3	0,173	0,1	<input style="width: 50px;" type="text" value="0"/>	0,199	0,231
Ethane	C2	6,01	0,0301	0,04	<input style="width: 50px;" type="text" value="0"/>	0,05	0,832
Propane	C3	3	0,015	0,04	<input style="width: 50px;" type="text" value="0"/>	0,0427	1,42
iso-Butane	iC4	1,1	0,0055	0,04	<input style="width: 50px;" type="text" value="0"/>	0,0404	3,67
n-Butane	nC4	0,9	0,009	0,04	<input style="width: 50px;" type="text" value="0"/>	0,041	4,56
iso-Pentane	iC5	0,35	0,0035	0,04	<input style="width: 50px;" type="text" value="0"/>	0,0402	11,5
n-Pentane	nC5	0,25	0,0025	0,04	<input style="width: 50px;" type="text" value="0"/>	0,0401	16
Hexane	C6	0,1	0,005	0,04	<input style="width: 50px;" type="text" value="0"/>	0,0403	40,3
Heptane	C7	0	0	0	<input style="width: 50px;" type="text" value="0"/>	0	0
Octane	C8	0	0	0	<input style="width: 50px;" type="text" value="0"/>	0	0
Nonane	C9	0	0	0	<input style="width: 50px;" type="text" value="0"/>	0	0
Decane	C10	0	0	0	<input style="width: 50px;" type="text" value="0"/>	0	0
Nitrogen	N2	1	0,005	0,04	<input style="width: 50px;" type="text" value="0"/>	0,0403	4,03
Carbon Dioxide	CO2	1	0,005	0,04	<input style="width: 50px;" type="text" value="0"/>	0,0403	4,03
Water	H2O	0	0	0	<input style="width: 50px;" type="text" value="0"/>	0	0
Hydrogen Sulphide	H2S	0	0	0	<input style="width: 50px;" type="text" value="0"/>	0	0
Hydrogen	H2	0	0	0	<input style="width: 50px;" type="text" value="0"/>	0	0
Carbon Monoxide	CO	0	0	0	<input style="width: 50px;" type="text" value="0"/>	0	0
Oxygen	O2	0	0	0	<input style="width: 50px;" type="text" value="0"/>	0	0
Helium	He	0	0	0	<input style="width: 50px;" type="text" value="0"/>	0	0
Argon	Ar	0	0	0	<input style="width: 50px;" type="text" value="0"/>	0	0

Figure 8.7 Input of uncertainties for gas analysis when “sampling” (with GC) is selected.

Fiscal Gas Metering Station Uncertainty v1.0.0 About Feedback

metering station conditions **gas analysis** flow meas results charts report

GC Analysis **Gas Properties**

Z specification: AGA8 0,1 Z_o specification: ISO 6976 0,0522

Uncertainty in CO₂ Emission Factors, Calorific Value and additional gas properties

Name	Value	Unit	Confidence	Documentation
CO ₂ Emission Factor in kg/kg	0,09	%	95%	
CO ₂ Emission Factor in kg/Sm ³	0,29	%	95%	
CO ₂ Emission Factor in tonnes/TJ	0,06	%	95%	
Sup. Calorific Value in MJ/kg	0,11	%	95%	
Inf. Calorific Value in MJ/kg	0,11	%	95%	
Molar mass in g/mol	0,25	%	95%	Note that the NORSOK I-106 requirement is 0.20 %

Gas Analysis, Density

Uncertainty in Density due to model, line conditions and gas composition uncertainties

Input Variable	Symbol	Uncertainty	Unit	Confidence	Std. Uncert. u _i	Sens. Coeff. s _i	Variance (s _i · u _i) ²
Pressure	P	0,3	%	Norm95	0,15 %	1	0,0225 % ²
Temperature	T	0,09284	%	Norm95	0,04642 %	1	0,002155 % ²
m/Z factor	m/Z	0,4056	%	Norm95	0,2028 %	1	0,04113 % ²
Sum of variances, $\sum (s_i \cdot u_i)^2$							0,06578 % ²
Relative Combined Standard Uncertainty							0,2565 %
Relative Expanded Uncertainty (95% Confidence level, k=2)							0,513 %

Gas Analysis, Z_o/√mZ factor

Uncertainty in Z_o/√mZ factor due to model, line conditions and gas composition uncertainties

Input Variable	Symbol	Uncertainty	Unit	Confidence	Std. Uncert. u _i	Sens. Coeff. s _i	Variance (s _i · u _i) ²
Z _{o,mod}	Z _{o,mod}	0,0522	%	Norm95	0,0261 %	1	0,0006812 % ²
Z _{mod}	Z _{mod}	0,1	%	Norm95	0,05 %	0,5	0,000625 % ²
Z _o /√mZ _{ana}		0,08027	%	Norm95	0,04014 %	1	0,001611 % ²
Sum of variances, $\sum (s_i \cdot u_i)^2$							0,002917 % ²
Relative Combined Standard Uncertainty							0,05401 %

Figure 8.8 Computed uncertainties of some important factors used in the models of the flow measurement uncertainties. In addition, the section contains user controls for selecting model standards for Z and Z_o.

8.3.4 Flow Measurement Page

The flow measurement page encompasses specification of uncertainty in instruments and other facilities used for flow measurement (Figure 8.9). Simple instruments like a temperature transmitter has one section for uncertainty specification, but more complex instruments like an orifice flow meter have several sections (as can be seen in Figure 8.9). Some instruments also include flow calibration data (Figure 8.10). Note that it can be selected how the meter is adjusted for the calibration curve, as described in Appendix A.

Depending on the equipment there can be functionality for using values from different standard specifications, as shown in Figure 8.9 where the user can select “ISO 5167 Specification” for the uncertainty in the orifice meter pipe diameter. An overall level can also be selected as the total uncertainty may depend on design, operational and maintenance routines designed to keep

measurements within a given maximum uncertainty. The uncertainty requirements in the Norwegian measurement regulations has been pre entered as default values. Some instruments have possibility for a detailed specification, as shown in Figure 8.11.

Fiscal Gas Metering Station Uncertainty v1.0.0 [About](#) [Feedback](#)

[metering station](#) [conditions](#) [gas analysis](#) [flow meas](#) [results](#) [charts](#) [report](#)

Orifice Meter Pipe Diameter Orifice Meter Orifice Diameter Orifice Meter Discharge Coeff. Orifice Meter Diff. Pressure Line Conditions Temperature Line Conditions Pressure Line Conditions Densitometer Densitometer Temperature

Orifice Meter, Pipe Diameter
☒ ISO 5167 Specification

Properties and Constants

Pipe Diameter mm

Input Variable	Uncertainty	Unit	Confidence	Std. Uncert. u_i	Sens. Coeff. s_i	Variance ($s_i \cdot u_i$) ²
Uncertainty	0,4	%	Norm95	0,6 mm	1	0,36 (mm) ²
Sum of variances, $\Sigma (s_i \cdot u_i)^2$						0,36 (mm) ²
Combined Standard Uncertainty, U_c						0,6 mm
Expanded Uncertainty (95% Confidence level, $k=2$), $k \cdot U_c$						1,2 mm
Value						300 mm
Relative Expanded Uncertainty (95% Confidence level, $k=2$)						0,4 %

0,4 % according to ISO 5167 Part 2 chapter 5.3.3.2

Figure 8.9 Flow measurement page for a template with orifice flow meter.

Fiscal Gas Metering Station Uncertainty v1.0.0 [About](#) [Feedback](#)

[metering station](#) [conditions](#) [gas analysis](#) [flow meas](#) [results](#) [charts](#) [report](#)

Flow Meter Lab Calibration Flow Meter Field Uncertainty Line Conditions Temperature Line Conditions Pressure Line Conditions Densitometer Densitometer Temperature

Flow Meter, Lab Calibration

[Add Calibration Point](#) [Remove Last Point](#) Correction:

Properties and Constants

Line pressure at cal. Pfc bara

Line temperature at cal. Tfc °C

#	Rate m ³ /h	Deviation (Uncorrected) %	Lab. Reference %, 95% Conf.	Repeatability %, 95% Conf.	Total %, 95% Conf.
1	106,916	1,2	0,2	0,1	0,224
2	267,292	0,55	0,2	0,1	0,224
3	668,231	0,3	0,2	0,1	0,224
4	1069,16	0,23	0,2	0,1	0,224
5	1871,04	0,18	0,2	0,1	0,224
6	2672,92	0,2	0,2	0,1	0,224
7	3474,80	0,24	0,2	0,1	0,224

comments/documentation

Figure 8.10 Flow measurement page for a template with ultrasonic flow meter. Note that the method for adjusting (correcting) the flow meter after calibration is to be specified here. See also Appendix A.

Fiscal Gas Metering Station Uncertainty v1.0.0 [About](#) [Feedback](#)

metering station conditions gas analysis **flow meas** results charts report

Flow Meter Lab Calibration Flow Meter Field Uncertainty Line Conditions Temperature **Line Conditions Pressure** Line Conditions Densitometer Densitometer Temperature

Line Conditions, Pressure

☐ Overall Input Level

Properties and Constants

Max Calibrated Static Pressure	<input type="text" value="120"/>	barg
Min Calibrated Static Pressure	<input type="text" value="50"/>	barg
Upper Range Limit	<input type="text" value="138"/>	barg
Time Between Calibrations	<input type="text" value="12"/>	Months
Ambient Temp At Calibration	<input type="text" value="20"/>	°C

Input Variable	Uncertainty	Unit	Confidence	Std. Uncert. u_i	Sens. Coeff. s_i	Variance $(s_i \cdot u_i)^2$
Transmitter	<input type="text" value="0,05"/>	%Span	99% (norm) ▼	0,01167 bara	1	0,0001361 (bara) ²
Stability	<input type="text" value="0,1"/>	%URL/yr	95% (norm) ▼	0,069 bara	1	0,004761 (bara) ²
RFI Effects	<input type="text" value="0,1"/>	%Span	99% (norm) ▼	0,02333 bara	1	0,0005444 (bara) ²
Ambient temp. effect	<input type="text" value="0,03"/>	%Span/28C	99% (norm) ▼	0,005 bara	1	2,5E-05 (bara) ²
Atmospheric pressure	<input type="text" value="0,09"/>	bar	99% (norm) ▼	0,03 bara	1	0,0009 (bara) ²
Misc.	<input type="text" value="0"/>	bar	95% (norm) ▼	0 bara	1	0 (bara) ²
Sum of variances, $\Sigma (s_i \cdot u_i)^2$						0,006367 (bara) ²
Combined Standard Uncertainty, U_c						0,07979 bara
Expanded Uncertainty (95% Confidence level, $k=2$), $k \cdot U_c$						0,1596 bara
Value						100 bara
Relative Expanded Uncertainty (95% Confidence level, $k=2$)						0,1596 %

Figure 8.11 Detailed input for a pressure transmitter.

8.3.5 Uncertainty Calculation Results Page

This page is the first of several pages that displays the result of the uncertainty calculation based on the input data (Figure 8.12). There is one section for each of the main flow measurement variables, standard volume flow, mass flow and energy flow. Depending on template there can be sections for additional measurements. For example, if the template included ultrasonic flow meter together with using GC for gas analysis, there is a section for the density measurement.

The uncertainty is displayed as uncertainty budgets tables, and the functional relationship is displayed for reference. Depending on the selected metering template, there can also be a list of “computed values”. These are values computed from the input data for use in the uncertainty calculation and listed here for convenience.

It is also possible to copy all or part of the tables in Figure 8.12 to Excel as a table. Select range with left mouse button pressed and use standard copy and paste operation into an Excel spreadsheet.

Fiscal Gas Metering Station Uncertainty

v1.0.0 [About](#) [Feedback](#)

metering station conditions gas analysis flow meas **results** charts report

USM Meter, Standard Volume Flow

$$q_{v0} = \frac{PT_0 Z_0}{P_0 T Z} q_v$$

Input Variable	Symbol	Uncertainty	Unit	Confidence	Std. Uncert. u_i	Sens. Coeff. s_i	Variance ($s_i \cdot u_i$) ²
Calib. Reference		0,2	%	Norm95	0,1 %	1	0,01 % ²
Calib. Repeatability		0,1	%	Norm95	0,05 %	1	0,0025 % ²
Calib. Deviation		0,02366	%	Norm95	0,01183 %	1	0,00014 % ²
Field Uncertainty		0,2	%	Norm95	0,1 %	1	0,01 % ²
Pressure	P	0,1596	%	Norm95	0,07979 %	1	0,006367 % ²
Temperature	T	0,04733	%	Norm95	0,02366 %	1	0,00056 % ²
Z/Z ₀ factor	Z/Z ₀	0,1219	%	Norm95	0,06093 %	1	0,003713 % ²
Sum of variances, $\Sigma (s_i \cdot u_i)^2$							0,03328 % ²
Relative Combined Standard Uncertainty							0,1824 %
Relative Expanded Uncertainty (95% Confidence level, k=2)							0,3649 %

USM Meter, Mass Flow

$$q_m = \rho q_v$$

Input Variable	Symbol	Uncertainty	Unit	Confidence	Std. Uncert. u_i	Sens. Coeff. s_i	Variance ($s_i \cdot u_i$) ²
Calib. Reference		0,2	%	Norm95	0,1 %	1	0,01 % ²
Calib. Repeatability		0,1	%	Norm95	0,05 %	1	0,0025 % ²
Calib. Deviation		0,02366	%	Norm95	0,01183 %	1	0,00014 % ²
Field Uncertainty		0,2	%	Norm95	0,1 %	1	0,01 % ²
Densitometer	ρ	0,2037	%	Norm95	0,1018 %	1	0,01037 % ²
Sum of variances, $\Sigma (s_i \cdot u_i)^2$							0,03301 % ²
Relative Combined Standard Uncertainty							0,1817 %
Relative Expanded Uncertainty (95% Confidence level, k=2)							0,3634 %

USM Meter, Energy Flow

$$q_e = H_s \rho q_v$$

Input Variable	Symbol	Uncertainty	Unit	Confidence	Std. Uncert. u_i	Sens. Coeff. s_i	Variance ($s_i \cdot u_i$) ²
Calib. Reference		0,2	%	Norm95	0,1 %	1	0,01 % ²

Figure 8.12 Computed uncertainty of the main flow measurement variables (standard volume flow, mass flow and energy flow) displayed as uncertainty budgets tables. It is possible to select range with left mouse button pressed and use standard copy and paste operation into an Excel spreadsheet.

8.3.6 Uncertainty Budget Charts Page

This page displays the computed uncertainty of the main flow measurement variables (standard volume flow, mass flow and energy flow) displayed as uncertainty budgets charts (Figure 8.13). Depending on template it also contains charts for other essential equipment, for example densitometer. The bar chart displays numerical values when the mouse pointer hover over a bar, and it is possible to copy the chart as an image by “right-clicking” on the chart and select either save or copy from the context menu.

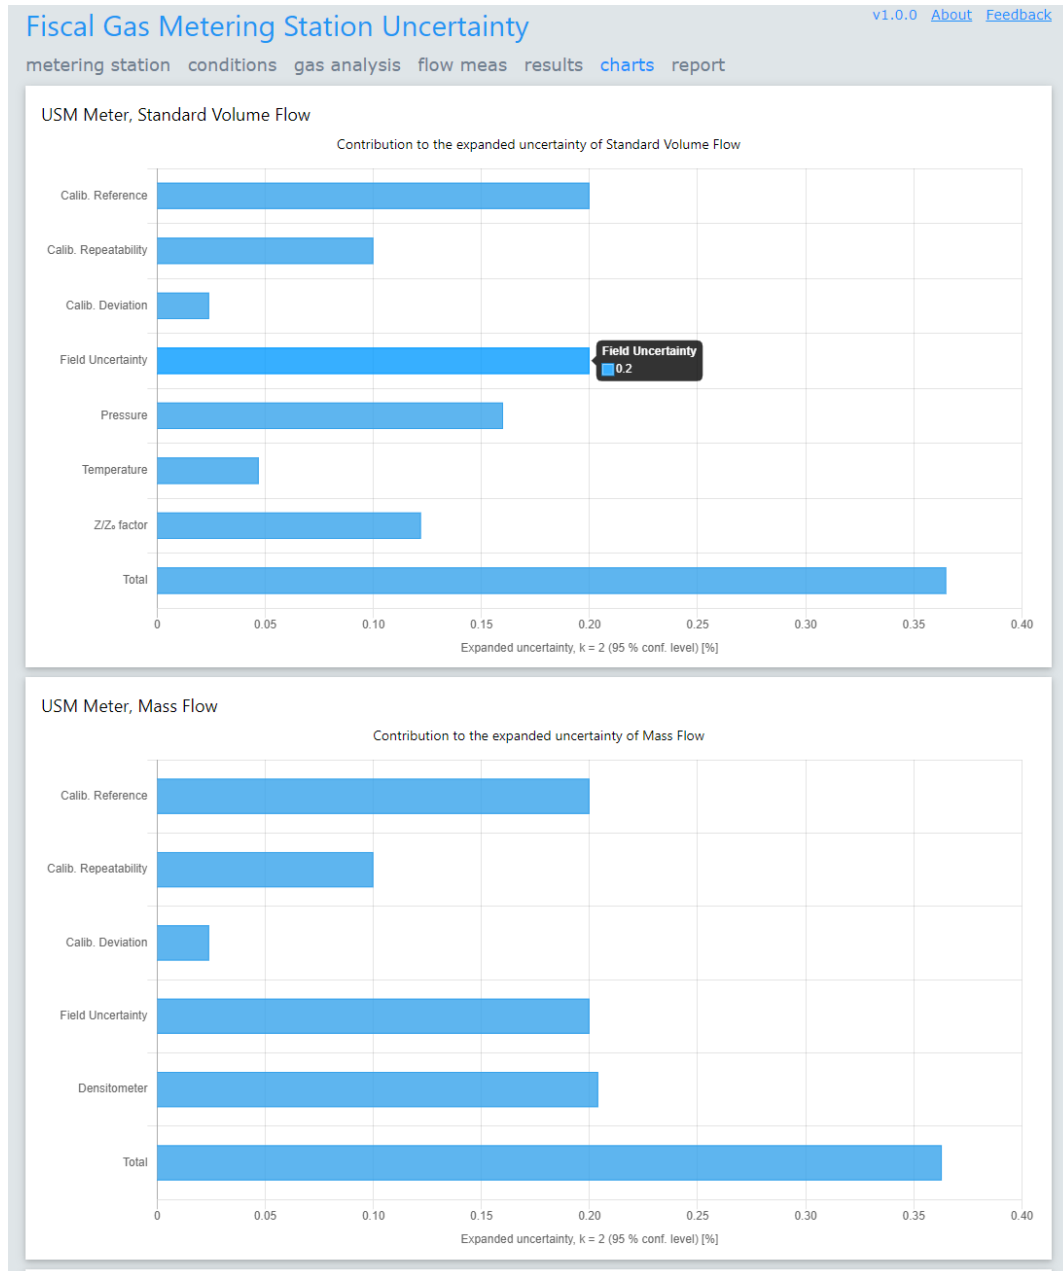


Figure 8.13 Computed uncertainty of the main flow measurement variables and equipment displayed as uncertainty budgets charts. Note that it is possible to copy the chart as an image by “right-clicking” on the chart and select either save or copy from the context menu.

8.3.7 Uncertainty Report Page

This page contains a summary of the uncertainty analysis formatted as an on-screen report (Figure 8.14). This can be printed, and it is also possible to save the analysis in an encrypted file for later use and reference.

- Print-button: shows the browser/system “print-preview” dialog where typical settings for the printout is selected, and a preview of the result is displayed.
- Save-button: downloads a file with a name consisting of the “name” and “date” fields selected on the frontpage of the application. If name is not specified, the string “gasmet” will be used as name.

The report includes the following:

- Header which integrates the <Name>, <Date> and <Description> input from start page.
- Graphic that displays the selected metering station template.
- Tables listing the line operating conditions.
- Table listing the computed gas properties according to AGA 8, AGA 10 and ISO 6976.
- Uncertainty budget for standard volume flow at the given flow rate in units of Sm^3/h . The functional relationship is displayed together with any relevant computed values used in the model.
- Uncertainty budget for mass flow at the given flow rate in units of kg/h . The functional relationship is displayed together with any relevant computed values used in the model.
- Uncertainty budget for energy flow at the given flow rate in units of GJ/h . The functional relationship is displayed together with any relevant computed values used in the model.
- Uncertainty budget for additional measurements, depending on template. For example if the template included ultrasonic flow meter together with using GC for gas analysis, there is an uncertainty budget for the density measurement.
- Uncertainty in CO_2 emission factors and calorific value.

Regarding printing, all recently updated operating systems have good support for printing HTML-pages directly and with high quality. The report page also has special formatting codes that will be used when the page is sent to the printer. One of them is “page-breaks” between sections so that tables and figures will be placed reasonably and, if possible, not split between pages.

The same functionality used for printing can be used together with a “print to pdf file”-driver that can be installed on the operating system. There are several suppliers of these drivers, and some operating systems have these installed as default (for example Windows 10). When using “print to pdf file”, the resulting pdf file will be in a format that allows selecting tables and values for copying to other applications for further use.

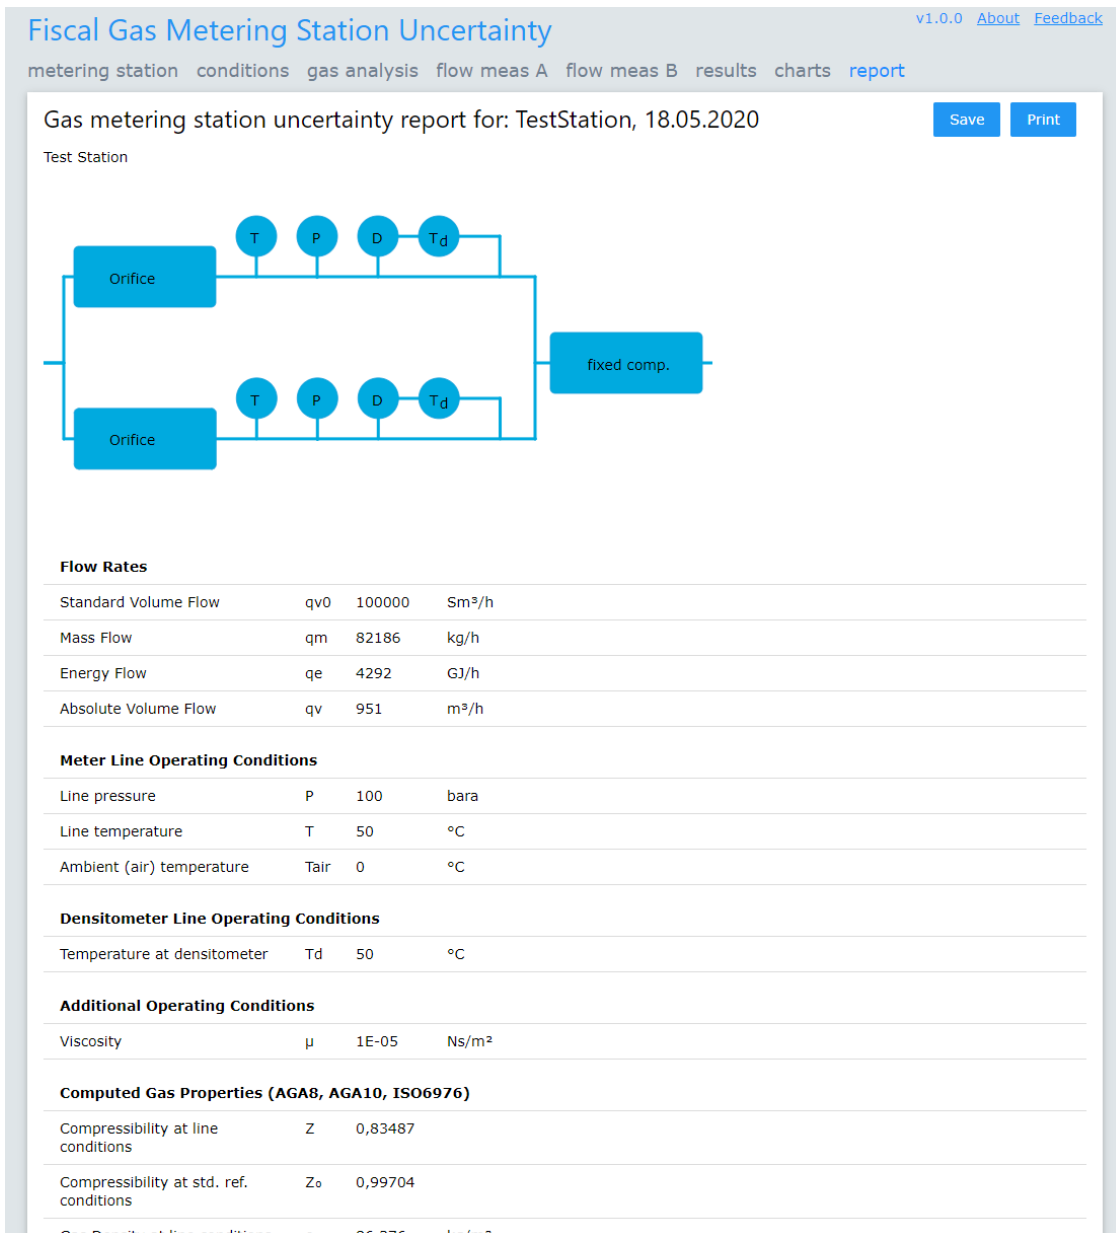


Figure 8.14 Report page contains a summary of the uncertainty analysis formatted as an on-screen report. This can be printed, and it is also possible to save the analysis in an encrypted file for later use and reference.

8.3.8 Note about use of “browser refresh”

The application holds all input and results in memory until the user explicitly saves an uncertainty analysis to file. If the user presses the browser refresh button at any point before saving, all input and results are lost. There is no reason for the user to do this, other than by accident. A “browser refresh” should be avoided, and if the user wants to start a new uncertainty analysis, the “Create New”-button on the application start page should be used. Note that the web-applications is not influenced by network disconnects, since after the web-application is loaded there is no further communication with the webserver.

9 Summary

This report documents uncertainty models for fiscal gas metering stations using either orifice, Coriolis or ultrasonic flow meters. The uncertainty models covers the case when a gas chromatograph is used, the case with gas sampling and the case with densitometer and a given gas composition. Two meters in parallel is covered, and for ultrasonic and Coriolis flow meters also two flow meters in series are covered. The uncertainty models are implemented on two different web-based platforms, one new web application (GasMetApp) using HTML and WebAssembly, and the original (GasMetering) using Microsoft Silverlight technology. Both versions use the same file format. These can be accessed for free from nfogm.no. Since support for the Silverlight runtime will end 12. October 2021, users should transition to the new web application before this date.

The present work is a generalization of the uncertainty models for fiscal gas metering stations in [Lunde et al, 2002] and [Dahl et al, 2003].

10 References

AGA 8: Starling, K.E. and Savidge, J.L.: "Compressibility Factors of Natural Gas and Other Related Hydrocarbon Gases," American Gas Association Transmission Measurement Committee Report No. 8, Arlington, USA, 1994 (2nd Printing).

AGA 10: "Speed of Sound in Natural Gas and Other Related Hydrocarbon Gases," American Gas Association Report No. 10, Prepared by Transmission Measurement Committee, Washington, USA, 2003.

ASTM D-1945, "Standard Test Method for Analysis of Natural Gas by Gas Chromatography," ASTM International standard No. D1945 – 03, West Conshohocken, USA, 2010.

Dahl, E., Frøysa, K.-E. and Lunde, P.: "Handbook of Uncertainty Calculations - Fiscal Orifice Gas and Turbine Oil Metering Stations", Issued by Norwegian Society for Oil and Gas Measurement (NFOGM) and Norwegian Petroleum Directorate, 2003.

ISO 5167-1, "Measurement of fluid flow by means of pressure differential devices inserted in circular cross-section conduits running full – Part 1: General principles and requirements," ISO, Geneva, 2003.

ISO 5167-2, "Measurement of fluid flow by means of pressure differential devices inserted in circular cross-section conduits running full – Part 2: Orifice plates," ISO, Geneva, 2003.

ISO 5168, "Measurement of fluid flow – Procedures for the evaluation of uncertainties," ISO. Geneva, 2005.

ISO 6976, "Natural gas – Calculation of calorific values, density, relative density and Wobbe index from composition," ISO, Geneva, 1995.

ISO 10790, "Measurement of fluid flow in closed conduits – Guidance to the selection, installation and use of Coriolis meters (mass flow, density and volume flow measurements," ISO, Geneva, 2015.

ISO 15970, "Natural gas – Measurement of properties – Volumetric properties: density, pressure, temperature and compression factor," ISO, Geneva, 2008.

ISO 17089-1, "Measurement of fluid flow in closed conduits – Ultrasonic meters for gas – Part 1: Meters for custody transfer and allocation measurement," ISO, Geneva, 2019.

ISO GUM, "Uncertainty of measurement – Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)," ISO guide 98-3, ISO, Geneva, 2008.

Lunde, P. and Frøysa, K.-E.: "Handbook of Uncertainty Calculations, ultrasonic fiscal gas metering stations," Issued by Norwegian Society for Oil and Gas Measurement (NFOGM) and Norwegian Petroleum Directorate, 2002.

Lunde, P., Frøysa, K.-E., Lied, G., Skatvedt, R. and Vervik, S.: "Handbook of uncertainty calculations. Fiscal oil metering stations based on ultrasonic duty and master meters," in proceedings from the 28th International North Sea Flow Measurement Workshop, St. Andrews, Scotland, October 2010.

NORSOK I-104: "Fiscal measurement system for hydrocarbon gas," NORSOK standard I-104, Rev. 3, November 2005.

NORSOK I-106: "Fiscal metering systems for hydrocarbon liquid and gas" NORSOK standard I-106, Edition 1, November 2014.

NPD, "Regulations relating to measurement of petroleum for fiscal purposes and for calculation of CO₂-tax (The measurement regulations)," The Norwegian Petroleum Directorate (NPD), 2001, last translated 2012.

Appendix A Detailed formulas for uncertainty of correction factor after flow calibration

This Appendix gives the details regarding the uncertainty of the correction factor estimate as an uncertainty contribution to the calibration uncertainty of a flow calibrated flow meter. It is related to the Coriolis flow meter functional relationship in Section 5.2.1 and uncertainty model in Section 5.3.1. More specifically it gives the value for the first term of the right hand side of Eq. (5.4). For ultrasonic flow meters, it is related to the functional relationship in Section 6.2.1 and uncertainty model in Section 6.3.1. More specifically it gives the value for the first term of the right hand side of Eq. (6.9).

The Coriolis flow meter is calibrated on mass flow rate, as this is the primary output of the Coriolis flow meter. Similarly, the ultrasonic flow meter is calibrated on actual volume flow rate. The method described here is similar for both types of flow meters and flow rates, and will be covered together. Thus, the following notation is used for the flow rates: index “ x ” can mean either “ m ” for mass or “ v ” for actual volume. In addition, the index “ $Meter$ ” will mean either “*Coriolis*” or “*USM*”, depending on the meter type in question.

The results presented here are based in [Lunde et al, 2002] and [Lunde et al, 2010].

A 1 Functional relationship

After flow calibration, an adjustment of the flow meter may be carried out. The flow calibration is carried by comparing the output flow rate from the flow meter with the similar reading from a reference measurement. This is carried out at a set of N different flow rates where the reference meter measured the flow rate $q_{x,ref,i}$ and the flow meter measured the flow rate $q_{x,Meter,i}$, $i = 1, \dots, N$. A full correction of the flow meter at each of these flow rates can therefore be written as

$$q_{x,i} = K_i q_{x,Meter,i}, \quad (A.1)$$

where

$$K_i = \frac{q_{x,ref,i}}{q_{x,Meter,i}}. \quad (A.2)$$

The relative difference in per cent between the flow rate as measured by the flow meter and the reference meter can be written as

$$p_i = 100 \frac{q_{x,Meter,i} - q_{x,ref,i}}{q_{x,ref,i}}. \quad (A.3)$$

The relation between these two quantities is

$$p_i = 100 \frac{1 - K_i}{K_i}; \quad K_i = \frac{100}{100 + p_i}. \quad (A.4)$$

From these correction factors a general correction factor valid for all flow rates (and not only at the specific flow rates where the flow calibration is carried out) is established. This can formally be written as

$$q_x = K q_{x,Meter}, \quad (A.5)$$

where

$$K = f(K_1, K_2, \dots, K_N, q_x). \quad (A.6)$$

This factor corresponds to correcting a percentage deviation of p %, where

$$p = 100 \frac{1-K}{K}; \quad K = 100/(100 + p). \quad (A.7)$$

In practice, such a correction can be carried out in different ways, including

- (i) no correction,
- (ii) a constant percentage correction,
- (iii) linear interpolation, and
- (iv) other methods (splines and other curve fittings).

In this report the three first methods will be covered.

In the first case, with no correction, K will be equal to one, and $p = 0$. The flow meter is then not adjusted to give the same output flow rate as the reference meter.

In the second case, an average percentage difference, $p = p_{corr}$, for example the flow weighted mean error, between the flow meter output and the reference measurement is established. Then a correction factor $K = 100/(100 + p_{corr})$ is established and used for all flow rates. It should be commented that in case (ii), the output flow rate of the flow meter after adjustment will generally not be the same as the flow rate measured by the reference instrumentation (for the flow rates used in the flow calibration). Thus, there will remain some known systematic errors in the flow meter. It should also be commented that case (i) is a special case of case (ii), with $p_{corr} = p = 0$.

In the third case, the adjustment will be based on a linear interpolation between the adjustment factors established for the flow rates used in the flow calibration. Such an interpolation can be carried out either on K , or on the percentage deviation p . Here, a linear interpolation in p is described. Both for the correction and for the uncertainty analysis, the results will almost be the same whether the interpolation is carried out on p or on K . The linear interpolation can be written as

$$p = p_i + \frac{p_{i+1} - p_i}{q_{x,Meter,i+1} - q_{x,Meter,i}} (q_{x,Meter} - q_{x,Meter,i}), \quad (A.8)$$

$$\text{when } q_{x,Meter,i} < q_{x,Meter} < q_{x,Meter,i+1}.$$

K can then be found from Eq. (A.7). It should be commented that this third case provides a correction such that the flow meter's flow rate will be corrected to the reference meter flow rate, when the flow rate is equal to any of the flow rates used in the flow calibration. This case is therefore in agreement with the Norwegian Petroleum Directorate Measurement Regulations, where one requirement in Section 8 is that "The measurement system shall be designed so that systematic measurement errors are avoided or compensated for". Using case (i) and (ii) is not in agreement with this requirement.

The fourth case is a generalization of the third case, where the linear interpolation is replaced with a non-linear interpolation (e.g. based on splines) or a partially linear interpolation where more interpolation

points than the ones used in the flow calibration (ref. case (iii)) are used. In such cases, it is recommended that for the uncertainty analysis, it is treated as case (iii).

A 2 Uncertainty model

The uncertainty of the flow rate due to the above mentioned adjustment of a flow meter after flow calibration will now be described. This is part of the of the calibration uncertainty described for Coriolis flow meters in Section 5.3.1 and for ultrasonic flow meters in Section 6.3.1. The uncertainty contribution is denoted “Uncertainty of the correction factor estimate”, and can be written as

$$\left(\frac{u(q_{x,cal,dev})}{q_x} \right)^2 = \left(\frac{u(K)}{K} \right)^2. \quad (A.9)$$

with a reference to Eq. (A.5). The term is related to the percentage difference, p , between flow rate from the flow meter and the reference measurement, because of Eq. (A.4). The actual expression depends on the adjustment method for the flow meter, and of any uncorrected percentage deviations, δp , between the flow meter and the reference meter. As discussed above, three adjustment methods will be addressed:

- (i) no correction,
- (ii) a constant percentage correction,
- (iii) linear interpolation.

Method (i): When no correction is done based on the deviation between the flow meter under calibration and the reference meter, all deviation is uncorrected. Because the flow meter then will have a known systematic deviation, such a procedure is not in accordance with e.g. the Norwegian Petroleum Directorate Measurement Regulations. However, such a lack of adjustment must contribute to additional uncertainty. The uncorrected percentage deviation therefore is found as linear interpolation as

$$\delta p = |p_i| + \frac{|p_{i+1}| - |p_i|}{q_{x,Meter,i+1} - q_{x,Meter,i}} (q_{x,Meter} - q_{x,Meter,i}), \quad (A.10)$$

$$\text{when } q_{x,Meter,i} < q_{x,Meter} < q_{x,Meter,i+1}.$$

For flow rates outside the calibrated range, extrapolation is carried out for getting an estimate for the uncorrected percentage deviation. In this case, the uncorrected percentage deviation increases as the flow rate leaves the calibrated range, and is calculated as

$$\delta p = |p_1| - \frac{|p_2| - |p_1|}{q_{x,Meter,2} - q_{x,Meter,1}} (q_{x,Meter} - q_{x,Meter,1}), \quad (A.11)$$

$$\text{when } q_{x,Meter} < q_{x,Meter,1},$$

and

$$\delta p = |p_n| + \frac{|p_n| - |p_{n-1}|}{q_{x,Meter,n} - q_{x,Meter,n-1}} (q_{x,Meter} - q_{x,Meter,n}); \quad (A.12)$$

$$\text{when } q_{x,Meter} > q_{x,Meter,n} .$$

Method (ii): When a constant percentage correction, p_{corr} , is carried out based on the deviation between the flow meter under calibration and the reference meter, there will be a remaining deviation between the adjusted flow meter and the reference meter. As for method (i) with no correction, there will strictly speaking be a known systematic deviation in the flow meter output. Therefore, such a procedure is not in accordance with e.g. the Norwegian Petroleum Directorate Measurement Regulations. However, such a lack of adjustment must contribute to additional uncertainty. The uncorrected percentage deviation therefore is found as linear interpolation as

$$\delta p = |p_i - p_{corr}| + \frac{|p_{i+1} - p_{corr}| - |p_i - p_{corr}|}{q_{x,Meter,i+1} - q_{x,Meter,i}} (q_{x,Meter} - q_{x,Meter,i}); \quad (A.13)$$

$$\text{when } q_{x,Meter,i} < q_{x,Meter} < q_{x,Meter,i+1} .$$

For flow rates outside the calibrated range, extrapolation is carried out for getting an estimate for the uncorrected percentage deviation. In this case, the uncorrected percentage deviation increases as the flow rate leaves the calibrated range, and is calculated as

$$\delta p = |p_1 - p_{corr}| - \frac{|p_2 - p_{corr}| - |p_1 - p_{corr}|}{q_{x,Meter,2} - q_{x,Meter,1}} (q_{x,Meter} - q_{x,Meter,1}); \quad (A.14)$$

$$\text{when } q_{x,Meter} < q_{x,Meter,1} ,$$

and

$$\delta p = |p_n - p_{corr}| + \frac{|p_n - p_{corr}| - |p_{n-1} - p_{corr}|}{q_{x,Meter,n} - q_{x,Meter,n-1}} (q_{x,Meter} - q_{x,Meter,n}); \quad (A.15)$$

$$\text{when } q_{x,Meter} > q_{x,Meter,n} .$$

Method (iii): The correction is carried out using a linear interpolation in the percentage deviation between the flow meter and the reference meter. The linear interpolation provides an approximate value for the deviation from reference for flow rates between the ones used in the flow calibration. This is illustrated in an example shown in Figure A.1, where a Coriolis flow meter is flow calibrated at mass flow rates of 5000 kg/h and 20000 kg/h. The deviation from reference at 5000 kg/h was 0.3 %. At 20000 kg/h it was 0.1 %. The blue curve represents the interpolated for mass flow rates between 5000 kg/h and 20000 kg/h. The correction of the meter is based on this curve. However, such a linear interpolation is an approximation, and the exact shape of the deviation curve is not known. In this work it is assumed that the true curve is somewhere inside the red parallelogram. It is further assumed that the probability is the same for the curve to be anywhere inside the parallelogram. The maximum (and unknown) uncorrected percentage deviation after correction is therefore not larger than:

When $q_{x,Meter,i} < q_{x,Meter} < \frac{q_{x,Meter,i} + q_{x,Meter,i+1}}{2}$:

$$\delta p = \frac{q_{x,Meter} - q_{x,Meter,i}}{q_{x,Meter,i+1} - q_{x,Meter,i}} |p_{i+1} - p_i|; \quad (A.16)$$

when $\frac{q_{x,Meter,i} + q_{x,Meter,i+1}}{2} < q_{x,Meter} < q_{x,Meter,i+1}$:

$$\delta p = \frac{q_{x,Meter,i+1} - q_{x,Meter}}{q_{x,Meter,i+1} - q_{x,Meter,i}} |p_{i+1} - p_i|. \quad (A.17)$$

This maximum percentage deviation is shown in Figure A.2.

For flow rates outside the calibrated range, extrapolation is carried out for getting an estimate for the uncorrected percentage deviation. In this case, the uncorrected percentage deviation increases as the flow rate leaves the calibrated range, and is calculated as

$$\delta p = -\frac{q_{x,Meter} - q_{x,Meter,1}}{q_{x,Meter,2} - q_{x,Meter,1}} |p_2 - p_1|; \quad (A.18)$$

when $q_{x,Meter} < q_{x,Meter,1}$,

and

$$\delta p = \frac{q_{x,Meter} - q_{x,Meter,n}}{q_{x,Meter,n} - q_{x,Meter,n-1}} |p_n - p_{n-1}|; \quad (A.19)$$

when $q_{x,Meter} > q_{x,Meter,n}$.

For all three types of correction (*Method (i)*, (*ii*) and (*iii*)), the expression for δp is considered to be expanded uncertainty of p with 100 % confidence level and rectangular distribution function. The standard uncertainty of p is then found by dividing δp with the square root of 3. The relative standard uncertainty of the correction factor estimate can now be written as

$$\left(\frac{u(q_{x,cal,dev})}{q_x} \right) = \left(\frac{u(K)}{K} \right) = \frac{1}{K} \frac{\partial p}{\partial K} u(p) = \frac{\delta p / \sqrt{3}}{100 + p}. \quad (A.20)$$

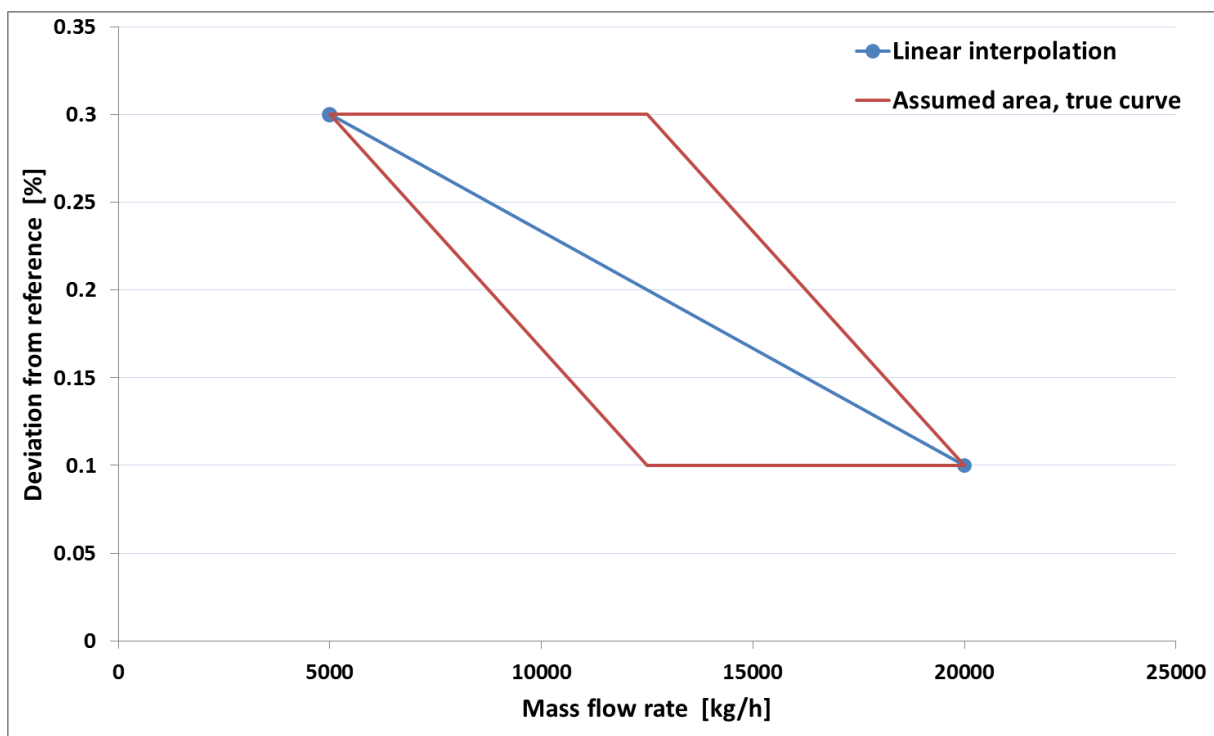


Figure A.1 Example of deviation from reference at flow calibration at a mass flow rate of 5000 kg/h (here deviation of 0.3 %) and 20000 kg/h (here deviation of 0.1%). For the correction of the flow meter, the deviation at flow rates between 5000 kg/h and 20000 kg/h are found by linear interpolation (blue curve). It is assumed that the “true” deviation curve is somewhere within the red parallelogram.

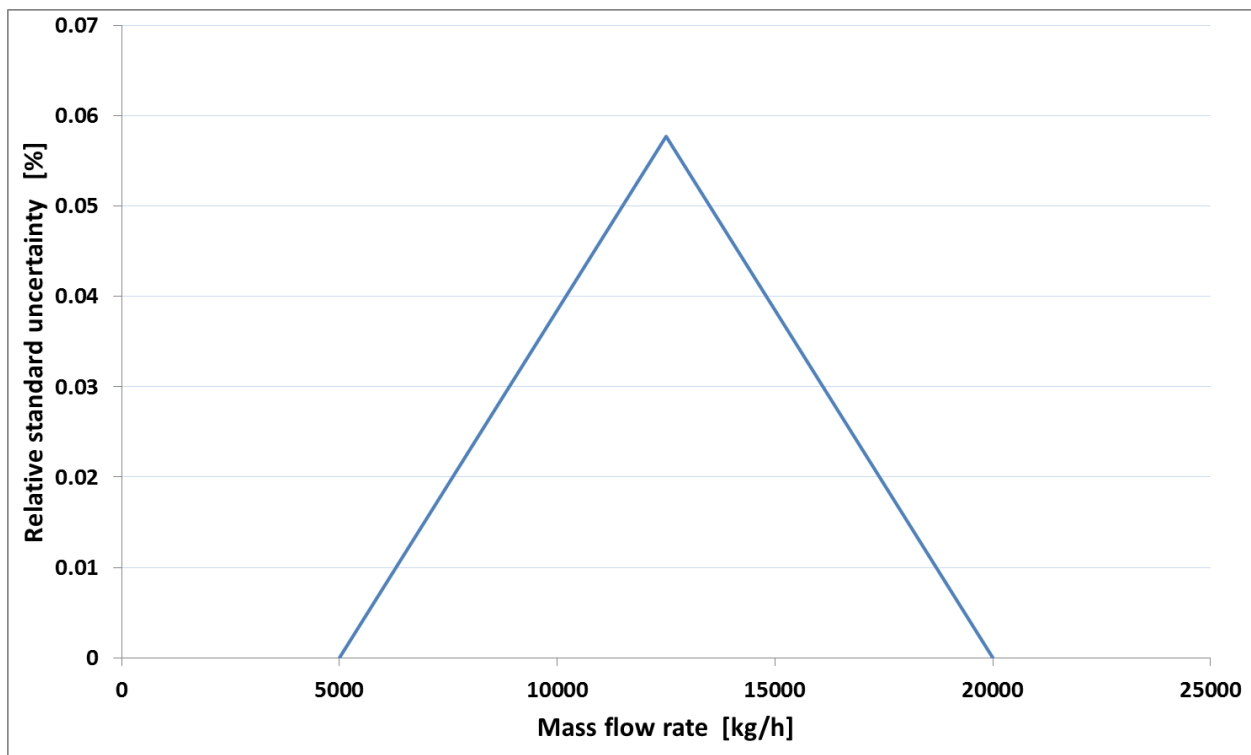


Figure A.2 Relative standard uncertainty related to the correction factor for the example shown in Figure A.1.

Appendix B Uncertainty model for two flow meters in parallel or in series

In this appendix, the uncertainty models for single flow meters are extended to cover two flow meters in parallel or two flow meters in series. First, a generic presentation for the uncertainty model for a single flow meter is presented. This result is thereafter used for development of uncertainty models for two meters in parallel or in series.

B 1 Generic uncertainty model for one flow meter

First, a generic uncertainty model for each of the two flow meters, meter A and meter B, is presented. It is shown here for mass flow rate, but can also be used for the other flow rates in question in this report.

The mass flow rate for each of the two meters (separately) can be found by the following generic equations:

$$\begin{aligned} q_{mA} &= f(x_{1A}, x_{2A}, \dots, x_{nA}), \\ q_{mB} &= f(x_{1B}, x_{2B}, \dots, x_{nB}). \end{aligned} \quad (\text{B.1})$$

As an example, if this is an orifice metering station, the equations correspond to Eqs. (4.4) or (4.7), depending on the set-up of the metering station. The x -variables correspond then to the various inputs to these equations, like discharge coefficient, expansibility coefficient, differential pressure, pressure, temperature, density and other gas parameters. n is 7 if densitometer is used and 8 elsewhere (by counting how many uncertainty contributions there are in Eqs. (4.4) and (4.7)). Similarly, there are influencing parameters also for the other types of flow meters.

The uncertainty model for each of these two flow rates can on absolute form be written as

$$u(q_{mA})^2 = \left(\frac{\partial f}{\partial x_1} u(x_{1A}) \right)^2 + \left(\frac{\partial f}{\partial x_2} u(x_{2A}) \right)^2 + \dots + \left(\frac{\partial f}{\partial x_n} u(x_{nA}) \right)^2, \quad (\text{B.2})$$

$$u(q_{mB})^2 = \left(\frac{\partial f}{\partial x_1} u(x_{1B}) \right)^2 + \left(\frac{\partial f}{\partial x_2} u(x_{2B}) \right)^2 + \dots + \left(\frac{\partial f}{\partial x_n} u(x_{nB}) \right)^2. \quad (\text{B.3})$$

This can be re-written to relative form by algebraic manipulations:

$$\left(\frac{u(q_{mA})}{q_{mA}} \right)^2 = \left(\frac{x_{1A}}{q_{mA}} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \right)^2 + \left(\frac{x_{2A}}{q_{mA}} \frac{\partial f}{\partial x_2} \frac{u(x_{2A})}{x_{2A}} \right)^2 + \dots + \left(\frac{x_{nA}}{q_{mA}} \frac{\partial f}{\partial x_n} \frac{u(x_{nA})}{x_{nA}} \right)^2, \quad (\text{B.4})$$

$$\left(\frac{u(q_{mB})}{q_{mB}} \right)^2 = \left(\frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{u(x_{1B})}{x_{1B}} \right)^2 + \left(\frac{x_{2B}}{q_{mB}} \frac{\partial f}{\partial x_2} \frac{u(x_{2B})}{x_{2B}} \right)^2 + \dots + \left(\frac{x_{nB}}{q_{mB}} \frac{\partial f}{\partial x_n} \frac{u(x_{nB})}{x_{nB}} \right)^2. \quad (\text{B.5})$$

If this is an orifice metering station, the equations correspond to Eqs. (4.10) or (4.13), depending on the set-up of the metering station. Note that each term on the right-hand-side of Eqs. (B.4) and (B.5)

represents the uncertainty contribution to the relative standard uncertainty of the mass flow rate in pipe A and B, respectively, originating from the uncertainty in each of the input parameters x_i .

B 2 Two flow meters in parallel

The total mass flow through the orifice metering station with two parallel runs, can now be written as

$$q_m = q_{mA} + q_{mB}. \quad (\text{B.6})$$

The uncertainty model for the total mass flow rate can on absolute form be written as

$$\begin{aligned} u(q_m)^2 = & \left(\frac{\partial f}{\partial x_1} u(x_{1A}) \right)^2 + \left(\frac{\partial f}{\partial x_1} u(x_{1B}) \right)^2 + 2r_1 \frac{\partial f}{\partial x_1} \frac{\partial f}{\partial x_1} u(x_{1A}) u(x_{1B}) \\ & + \left(\frac{\partial f}{\partial x_2} u(x_{2A}) \right)^2 + \left(\frac{\partial f}{\partial x_2} u(x_{2B}) \right)^2 + 2r_2 \frac{\partial f}{\partial x_2} \frac{\partial f}{\partial x_2} u(x_{2A}) u(x_{2B}) \\ & + \dots + \left(\frac{\partial f}{\partial x_n} u(x_{nA}) \right)^2 + \left(\frac{\partial f}{\partial x_n} u(x_{nB}) \right)^2 + 2r_n \frac{\partial f}{\partial x_n} \frac{\partial f}{\partial x_n} u(x_{nA}) u(x_{nB}). \end{aligned} \quad (\text{B.7})$$

In this formula, the concept of correlation has been addressed. In the uncertainty model for one single orifice meter, correlations have been avoided by the careful choice of input parameters. However, when considering two meters in parallel, similar measurements/calculations have been carried out for each run, and an evaluation on possible correlation between these measurements/calculations have to be made.

The correlation coefficient r_1 represents the correlation between the uncertainty in input parameter 1 (x_1) between pipe A and B. If there is full correlation, the correlation coefficient is 1. If there is no correlation, the correlation coefficient is 0. It is similar for the other input parameters (x_2 to x_n).

This can be re-written to relative form by algebraic manipulations:

$$\begin{aligned}
\left(\frac{u(q_m)}{q_m}\right)^2 &= \left(\frac{q_{mA}}{q_m} \frac{x_{1A}}{q_{mA}} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}}\right)^2 + \left(\frac{q_{mB}}{q_m} \frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{u(x_{1B})}{x_{1B}}\right)^2 \\
&+ 2r_1 \frac{q_{mA}}{q_m} \frac{q_{mB}}{q_m} \frac{x_{1A}}{q_{mA}} \frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \frac{u(x_{1B})}{x_{1B}} \\
&+ \left(\frac{q_{mA}}{q_m} \frac{x_{2A}}{q_{mA}} \frac{\partial f}{\partial x_2} \frac{u(x_{2A})}{x_{2A}}\right)^2 + \left(\frac{q_{mB}}{q_m} \frac{x_{2B}}{q_{mB}} \frac{\partial f}{\partial x_2} \frac{u(x_{2B})}{x_{2B}}\right)^2 \\
&+ 2r_2 \frac{q_{mA}}{q_m} \frac{q_{mB}}{q_m} \frac{x_{2A}}{q_{mA}} \frac{x_{2B}}{q_{mB}} \frac{\partial f}{\partial x_2} \frac{\partial f}{\partial x_2} \frac{u(x_{2A})}{x_{2A}} \frac{u(x_{2B})}{x_{2B}} \\
&+ \dots + \left(\frac{q_{mA}}{q_m} \frac{x_{nA}}{q_{mA}} \frac{\partial f}{\partial x_n} \frac{u(x_{nA})}{x_{nA}}\right)^2 + \left(\frac{q_{mB}}{q_m} \frac{x_{nB}}{q_{mB}} \frac{\partial f}{\partial x_n} \frac{u(x_{nB})}{x_{nB}}\right)^2 \\
&+ 2r_n \frac{q_{mA}}{q_m} \frac{q_{mB}}{q_m} \frac{x_{nA}}{q_{mA}} \frac{x_{nB}}{q_{mB}} \frac{\partial f}{\partial x_n} \frac{\partial f}{\partial x_n} \frac{u(x_{nA})}{x_{nA}} \frac{u(x_{nB})}{x_{nB}}.
\end{aligned} \tag{B.8}$$

Now assume that the flow in pipe A and B is of the same size. This means that $q_{mA}/q_m = q_{mB}/q_m = 1/2$. This simplifies the above equation:

$$\begin{aligned}
\left(\frac{u(q_m)}{q_m}\right)^2 &= \frac{1}{4} \left\{ \left(\frac{x_{1A}}{q_{mA}} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}}\right)^2 + \left(\frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{u(x_{1B})}{x_{1B}}\right)^2 \right. \\
&+ 2r_1 \frac{x_{1A}}{q_{mA}} \frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \frac{u(x_{1B})}{x_{1B}} \\
&+ \left(\frac{x_{2A}}{q_{mA}} \frac{\partial f}{\partial x_2} \frac{u(x_{2A})}{x_{2A}}\right)^2 + \left(\frac{x_{2B}}{q_{mB}} \frac{\partial f}{\partial x_2} \frac{u(x_{2B})}{x_{2B}}\right)^2 \\
&+ 2r_2 \frac{x_{2A}}{q_{mA}} \frac{x_{2B}}{q_{mB}} \frac{\partial f}{\partial x_2} \frac{\partial f}{\partial x_2} \frac{u(x_{2A})}{x_{2A}} \frac{u(x_{2B})}{x_{2B}} \\
&+ \dots + \left(\frac{x_{nA}}{q_{mA}} \frac{\partial f}{\partial x_n} \frac{u(x_{nA})}{x_{nA}}\right)^2 + \left(\frac{x_{nB}}{q_{mB}} \frac{\partial f}{\partial x_n} \frac{u(x_{nB})}{x_{nB}}\right)^2 \\
&\left. + 2r_n \frac{x_{nA}}{q_{mA}} \frac{x_{nB}}{q_{mB}} \frac{\partial f}{\partial x_n} \frac{\partial f}{\partial x_n} \frac{u(x_{nA})}{x_{nA}} \frac{u(x_{nB})}{x_{nB}} \right\}.
\end{aligned} \tag{B.9}$$

The correlation coefficients will as the model is used here be either 0 (uncorrelated) or 1 (fully correlated).

If the correlation coefficient $r_1 = 0$, the terms related to the x_1 variable (two first lines in the right hand side of Eq. (B.9)) will reduce to

$$\begin{aligned}
 & \frac{1}{4} \left\{ \left(\frac{x_{1A}}{q_{mA}} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \right)^2 + \left(\frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{u(x_{1B})}{x_{1B}} \right)^2 \right. \\
 & \left. + 2r_1 \frac{x_{1A}}{q_{mA}} \frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \frac{u(x_{1B})}{x_{1B}} \right\} \\
 & = \\
 & \frac{1}{4} \left\{ \left(\frac{x_{1A}}{q_{mA}} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \right)^2 + \left(\frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{u(x_{1B})}{x_{1B}} \right)^2 \right\}.
 \end{aligned} \tag{B.10}$$

Note that the two expressions in the parentheses in the last line of Eq. (B.10) are the uncertainty contributions to q_{mA} and q_{mB} , respectively, originating from the uncertainty in the input parameters x_{1A} and x_{1B} . This can be seen by comparing with Eqs. (B.4) and (B.5).

If the correlation coefficient $r_1 = 1$, the terms related to the x_1 variable (two first lines in the right hand side of Eq. (B.9)) will reduce to

$$\begin{aligned}
 & \frac{1}{4} \left\{ \left(\frac{x_{1A}}{q_{mA}} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \right)^2 + \left(\frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{u(x_{1B})}{x_{1B}} \right)^2 \right. \\
 & \left. + 2r_1 \frac{x_{1A}}{q_{mA}} \frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \frac{u(x_{1B})}{x_{1B}} \right\} \\
 & = \\
 & \frac{1}{4} \left\{ \left(\frac{x_{1A}}{q_{mA}} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} + \frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{u(x_{1B})}{x_{1B}} \right)^2 \right\}.
 \end{aligned} \tag{B.11}$$

Note that also here the uncertainty contributions to q_{mA} and q_{mB} , respectively, originating from the uncertainty in the input parameters x_{1A} and x_{1B} appear.

In order to apply this uncertainty model, the various uncertainty contributions have to be classified as either correlated or uncorrelated. This is done in the chapters covering the different flow meters.

In the derivation of the uncertainty model, the mass flow rate has been in focus. The standard volumetric flow rate and the energy flow rate can be treated in exactly the same way.

B 3 Two flow meters in series

The average mass flow found from the two flow meters, can now be written as

$$q_m = \frac{q_{mA} + q_{mB}}{2}. \tag{B.12}$$

The uncertainty model for the total mass flow rate can on absolute form be written as

$$\begin{aligned}
 u(q_m)^2 = \frac{1}{4} & \left\{ \left(\frac{\partial f}{\partial x_1} u(x_{1A}) \right)^2 + \left(\frac{\partial f}{\partial x_1} u(x_{1B}) \right)^2 + 2r_1 \frac{\partial f}{\partial x_1} \frac{\partial f}{\partial x_1} u(x_{1A}) u(x_{1B}) \right. \\
 & + \left(\frac{\partial f}{\partial x_2} u(x_{2A}) \right)^2 + \left(\frac{\partial f}{\partial x_2} u(x_{2B}) \right)^2 + 2r_2 \frac{\partial f}{\partial x_2} \frac{\partial f}{\partial x_2} u(x_{2A}) u(x_{2B}) \\
 & \left. + \dots + \left(\frac{\partial f}{\partial x_n} u(x_{nA}) \right)^2 + \left(\frac{\partial f}{\partial x_n} u(x_{nB}) \right)^2 + 2r_n \frac{\partial f}{\partial x_n} \frac{\partial f}{\partial x_n} u(x_{nA}) u(x_{nB}) \right\}.
 \end{aligned} \quad (B.13)$$

In this formula, like for two meters in parallel the concept of correlation has been addressed. In the uncertainty model for one single flow meter there are assumed to be no correlations. However, when considering two meters in series, similar measurements/calculations have been carried out for each run, and an evaluation on possible correlation between these measurements/calculations has to be made.

The correlation coefficient r_1 represents the correlation between the uncertainty in input parameter 1 (x_1) between meter A and B. If there is full correlation, the correlation coefficient is 1. If there is no correlation, the correlation coefficient is 0. It is similar for the other input parameters (x_2 to x_n).

This can be re-written to relative form by algebraic manipulations:

$$\begin{aligned}
 \left(\frac{u(q_m)}{q_m} \right)^2 = \frac{1}{4} & \left\{ \left(\frac{q_{mA}}{q_m} \frac{x_{1A}}{q_{mA}} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \right)^2 + \left(\frac{q_{mB}}{q_m} \frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{u(x_{1B})}{x_{1B}} \right)^2 \right. \\
 & + 2r_1 \frac{q_{mA}}{q_m} \frac{q_{mB}}{q_m} \frac{x_{1A}}{q_{mA}} \frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \frac{u(x_{1B})}{x_{1B}} \\
 & + \left(\frac{q_{mA}}{q_m} \frac{x_{2A}}{q_{mA}} \frac{\partial f}{\partial x_2} \frac{u(x_{2A})}{x_{2A}} \right)^2 + \left(\frac{q_{mB}}{q_m} \frac{x_{2B}}{q_{mB}} \frac{\partial f}{\partial x_2} \frac{u(x_{2B})}{x_{2B}} \right)^2 \\
 & + 2r_2 \frac{q_{mA}}{q_m} \frac{q_{mB}}{q_m} \frac{x_{2A}}{q_{mA}} \frac{x_{2B}}{q_{mB}} \frac{\partial f}{\partial x_2} \frac{\partial f}{\partial x_2} \frac{u(x_{2A})}{x_{2A}} \frac{u(x_{2B})}{x_{2B}} \\
 & + \dots + \left(\frac{q_{mA}}{q_m} \frac{x_{nA}}{q_{mA}} \frac{\partial f}{\partial x_n} \frac{u(x_{nA})}{x_{nA}} \right)^2 + \left(\frac{q_{mB}}{q_m} \frac{x_{nB}}{q_{mB}} \frac{\partial f}{\partial x_n} \frac{u(x_{nB})}{x_{nB}} \right)^2 \\
 & \left. + 2r_n \frac{q_{mA}}{q_m} \frac{q_{mB}}{q_m} \frac{x_{nA}}{q_{mA}} \frac{x_{nB}}{q_{mB}} \frac{\partial f}{\partial x_n} \frac{\partial f}{\partial x_n} \frac{u(x_{nA})}{x_{nA}} \frac{u(x_{nB})}{x_{nB}} \right\}.
 \end{aligned} \quad (B.14)$$

It is obvious that the same gas flows through both meters. Therefore for the purpose of an uncertainty model the following identities will be used: $q_{mA}/q_m = q_{mB}/q_m = 1$. This simplifies the above equation:

$$\begin{aligned}
 \left(\frac{u(q_m)}{q_m} \right)^2 &= \frac{1}{4} \left\{ \left(\frac{x_{1A}}{q_{mA}} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \right)^2 + \left(\frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{u(x_{1B})}{x_{1B}} \right)^2 \right. \\
 &\quad + 2r_1 \frac{x_{1A}}{q_{mA}} \frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \frac{u(x_{1B})}{x_{1B}} \\
 &\quad + \left(\frac{x_{2A}}{q_{mA}} \frac{\partial f}{\partial x_2} \frac{u(x_{2A})}{x_{2A}} \right)^2 + \left(\frac{x_{2B}}{q_{mB}} \frac{\partial f}{\partial x_2} \frac{u(x_{2B})}{x_{2B}} \right)^2 \\
 &\quad + 2r_2 \frac{x_{2A}}{q_{mA}} \frac{x_{2B}}{q_{mB}} \frac{\partial f}{\partial x_2} \frac{\partial f}{\partial x_2} \frac{u(x_{2A})}{x_{2A}} \frac{u(x_{2B})}{x_{2B}} \\
 &\quad + \dots + \left(\frac{x_{nA}}{q_{mA}} \frac{\partial f}{\partial x_n} \frac{u(x_{nA})}{x_{nA}} \right)^2 + \left(\frac{x_{nB}}{q_{mB}} \frac{\partial f}{\partial x_n} \frac{u(x_{nB})}{x_{nB}} \right)^2 \\
 &\quad \left. + 2r_n \frac{x_{nA}}{q_{mA}} \frac{x_{nB}}{q_{mB}} \frac{\partial f}{\partial x_n} \frac{\partial f}{\partial x_n} \frac{u(x_{nA})}{x_{nA}} \frac{u(x_{nB})}{x_{nB}} \right\}.
 \end{aligned} \tag{B.15}$$

Note that this equation is identical to Eq. (B.9). The correlation coefficients will as the model is used here be either 0 (uncorrelated) or 1 (fully correlated).

If the correlation coefficient $r_1 = 0$, the terms related to the x_1 variable (two first lines in the right hand side of Eq. (B.15)) will reduce to

$$\begin{aligned}
 &\frac{1}{4} \left\{ \left(\frac{x_{1A}}{q_{mA}} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \right)^2 + \left(\frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{u(x_{1B})}{x_{1B}} \right)^2 \right. \\
 &\quad \left. + 2r_1 \frac{x_{1A}}{q_{mA}} \frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \frac{u(x_{1B})}{x_{1B}} \right\} \\
 &= \\
 &\frac{1}{4} \left\{ \left(\frac{x_{1A}}{q_{mA}} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \right)^2 + \left(\frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{u(x_{1B})}{x_{1B}} \right)^2 \right\}.
 \end{aligned} \tag{B.16}$$

Note that the two expressions in the parentheses in the last line of Eq. (B.16) are the uncertainty contributions to q_{mA} and q_{mB} , respectively, originating from the uncertainty in the input parameters x_{1A} and x_{1B} . This can be seen by comparing with Eqs. (B.4) and (B.5).

If the correlation coefficient $r_1 = 1$, the terms related to the x_1 variable (two first lines in the right hand side of Eq. (B.16)) will reduce to

$$\begin{aligned}
& \frac{1}{4} \left\{ \left(\frac{x_{1A}}{q_{mA}} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \right)^2 + \left(\frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{u(x_{1B})}{x_{1B}} \right)^2 \right. \\
& \quad \left. + 2r_1 \frac{x_{1A}}{q_{mA}} \frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} \frac{u(x_{1B})}{x_{1B}} \right\} \\
& = \\
& \frac{1}{4} \left\{ \left(\frac{x_{1A}}{q_{mA}} \frac{\partial f}{\partial x_1} \frac{u(x_{1A})}{x_{1A}} + \frac{x_{1B}}{q_{mB}} \frac{\partial f}{\partial x_1} \frac{u(x_{1B})}{x_{1B}} \right)^2 \right\}.
\end{aligned} \tag{B.17}$$

Note that also here the uncertainty contributions to q_{mA} and q_{mB} , respectively, originating from the uncertainty in the input parameters x_{1A} and x_{1B} appear.

In order to apply this uncertainty model, the various uncertainty contributions have to be classified as either correlated or uncorrelated. This is done in the chapters covering the different flow meters.

In the derivation of the uncertainty model, the mass flow rate has been in focus. The standard volumetric flow rate and the energy flow rate can be treated in exactly the same way.

Appendix C USM field uncertainty, detailed level

In Section 6.3.2, the field uncertainty of a flow calibrated ultrasonic flow meter is discussed. One of the uncertainty contributions to the field uncertainty is the *uncertainty due to changes of conditions from flow calibration to field operation*. This is the last term in Eq. (6.11). As stated in the text, this term can either be given on an overall level or calculated from more detailed analysis of the ultrasonic flow meter. The more detailed analysis was developed in [Lunde et al, 2002] and is taken from there.

The specific link between [Lunde et al, 2002] and the present work is that Eq. (3.19) in [Lunde et al, 2002] corresponds to the Eq. (6.11) in this report:

$$\left(\frac{u(q_{v,field})}{q_{v,field}} \right)^2 = E_{USM}^2 \quad (C.1)$$

The first term on the right hand side of these two equations both covers the repeatability. The two last terms of Eq. (3.19) in [Lunde et al, 2002] will together cover the second and last term on the right hand side of Eq. (6.11). This means that

$$\left(\frac{u(q_{v,field,cond})}{q_{v,field,cond}} \right)^2 = E_{USM,\Delta}^2 + E_{misc}^2 \quad (C.2)$$

Here the left hand side is the symbol used in the present work, and found in Eq. (6.11), while the right hand side is taken from Eq. (3.19) in [Lunde et al, 2002].

In [Lunde et al, 2002] it is shown, see Eq. (3.20), that $E_{USM,\Delta}^2$ consists of three term, (i) related to meter body expansion due to pressure and temperature changes, (ii) related to changes in ultrasonic transit times and (iii) related to changes in flow profile (integration).

When this detailed level is chosen the following information is needed:

- Configuration:
 - Dimensions and Materials:
 - Inner diameter of meter spool
 - Average wall thickness
 - Temperature expansion coefficient
 - Youngs modulus of elasticity for meter spool
 - Acoustic paths:
 - Number of acoustic paths
 - Inclination angle of each acoustic path
 - Number of reflections for each acoustic path
 - Lateral chord position of each acoustic path
 - Integration weight factor of each acoustic path
- Repeatability (as for overall level)
- Meter body expansions:
 - Tick off whether pressure and temperature correction is carried out or not
 - Uncertainty of thermal expansion factor
 - Uncertainty of pressure expansion factor
- Transit time, installation and other effects:
 - Uncertainty in upstream time measurement
 - Uncertainty in downstream time measurement
- Integration uncertainty
- Miscellaneous uncertainty

Appendix D List of symbols

Common parameters

C_e :	CO ₂ emission factor pr energy unit (tonnes/TJ)
C_m :	CO ₂ emission factor pr mass unit (kg/kg)
C_v :	CO ₂ emission factor pr standard volume unit (kg/Sm ³)
$H_{I,m}$:	Inferior calorific value per mass
$H_{s,m}$:	Superior calorific value per mass
K :	Correction factor to be applied after flow calibration, see Eq. (A.5)
m :	Molar mass
p :	Percentage deviation that is corrected after flow calibration, see Eq. (A.7)
P :	Absolute pressure at line conditions
P_0 :	Absolute standard pressure (1 atm = 101325 Pa)
q_e :	Energy flow rate
q_m :	Mass flow rate
q_{v0} :	Standard volumetric flow rate (volumetric flow rate converted to standard temperature and pressure)
R :	Universal gas constant (8.31451 J/(mole K), ref [ISO 6976])
T :	Absolute temperature (Kelvin) at line conditions
T_0 :	Absolute standard temperature (288.15 K = 15 °C)
$u(X)$:	Standard uncertainty of quantity X
$u(X)/X$:	Relative standard uncertainty of quantity X
Z :	Gas compressibility at line conditions
Z_0 :	Gas compressibility at standard pressure and temperature
δp :	Uncorrected percentage deviation after flow calibration, see Section A 2.
ρ :	Gas density at line conditions
ρ_0 :	Gas density at standard conditions
ϕ_i :	Molar fraction of gas component number i

Subscripts “A” and “B” refer to meter A and B, respectively, when two flow meters in parallel or in series are addressed.

Parameters relevant for orifice metering station only

C :	Discharge coefficient
D :	Inner pipe diameter
d :	Orifice diameter
ΔP :	Differential pressure over the orifice plate
ε :	Expansibility coefficient

Subscript “1” corresponds to line conditions upstream of the orifice plate.

Subscript “2” corresponds to line conditions downstream of the orifice plate.

Parameters relevant for Coriolis metering station only

None

Parameters relevant for ultrasonic metering station only

q_v : Volumetric flow rate at line pressure and temperature